

# RayBio<sup>®</sup> Mouse TNF-Alpha IQELISA Kit

Catalog #: IQM-TNFA

User Manual

Last revised February 12, 2020

Caution:  
Extraordinarily useful information enclosed



ISO 13485 Certified

3607 Parkway Lane, Suite 100  
Norcross, GA 30092

Tel: 1-888-494-8555 (Toll Free) or 770-729-2992, Fax: 770-206-2393  
Web: [www.RayBiotech.com](http://www.RayBiotech.com), Email: [info@raybiotech.com](mailto:info@raybiotech.com)



RayBiotech, Inc.

---

## RayBio<sup>®</sup> Mouse TNF-Alpha IQELISA Kit Protocol

### Table of Contents

| Section |                               | Page # |
|---------|-------------------------------|--------|
| I.      | Introduction                  | 3      |
| II.     | Reagents                      | 3      |
| III.    | Storage                       | 3      |
| IV.     | Additional Materials Required | 4      |
| V.      | Reagent Preparation           | 4      |
| VI.     | Assay Procedure               | 5      |
| VII.    | Assay Procedure Summary       | 7      |
| VIII.   | Calculation of Results        | 8      |
|         | A. Typical Data               | 9      |
|         | B. Sensitivity and Recovery   | 9      |
| IX.     | Troubleshooting Guide         | 10     |

## I. INTRODUCTION

The RayBio® Immuno Quantitative Enzyme Linked ImumunoSorbent Assay (IQELISA) is an innovative new assay that combines the specificity and ease of use of an ELISA with the sensitivity of real-time PCR. This results in an assay that is simultaneously familiar and cutting edge and enables the use of lower sample volumes while also providing more sensitivity. The RayBio® Mouse TNF-Alpha IQELISA Kit is a modified ELISA assay with high sensitivity qPCR readout for the quantitative measurement of Mouse TNFa in serum, plasma, and cell culture supernatants. This assay employs an antibody specific for Mouse TNFa coated on a 96-well PCR plate. Standards and samples are pipetted into the wells and TNFa present in a sample is bound to the wells by the immobilized antibody. The wells are washed and a detection affinity molecule is added to the plates. After washing away unbound detection affinity molecule, primers and a PCR master mix are added to the wells and data is collected using qPCR.  $C_t$  values obtained from the qPCR are then used to calculate the amount of antigen contained in each sample, where lower  $C_t$  values indicate a higher concentration of antigen.

## II. REAGENTS

1. TNFa Microplate (Item A): 96-well PCR plate coated with anti-Mouse TNFa
2. Wash Buffer I Concentrate (20x) (Item B): 25 ml of 20x concentrated solution.
3. Standards (Item C): 2 vials of recombinant Mouse TNFa.
4. Assay Diluent A (Item D): 30 ml diluent buffer, 0.09% sodium azide as preservative.
5. Assay Diluent B (Item E): 15 ml of 5x concentrated buffer.
6. Detection Antibody for TNFa (Item F): 2 vials of a concentrated solution of anti-Mouse TNFa affinity reagent.
7. IQELISA Detection Reagent (Item G): 1.4ml of a 10x concentrated stock
8. Primer Solution (Item I): 1.7ml vial
9. PCR Master Mix (Item J): 1.2ml vial
10. PCR Preparation buffer (Item K): 1ml vial of 10x concentrated buffer
11. Final Wash Buffer (Item L): 10 ml vial of 10x concentrated buffer
12. PCR Caps

## III. STORAGE

May be stored for up to 6 months at 2° to 8° C from the date of shipment. Standard (recombinant protein) should be stored at -20° C or -80° C (recommended at -80° C) after reconstitution. Opened PCR plate or reagents may be stored for up to 1 month at 2° to 8° C. Note: the kit can be used within one year if the whole kit is stored at -20° C. Avoid repeated freeze-thaw cycles.

#### IV. ADDITIONAL MATERIALS REQUIRED

1. Real-time PCR instrument, Bio-Rad recommended
2. Precision pipettes to deliver 2µl to 1 ml volumes.
3. Adjustable 1-25 ml pipettes for reagent preparation.
4. 100 ml and 1 liter graduated cylinders.
5. Absorbent paper.
6. Distilled or deionized water.
7. Log-log graph paper or computer and software for data analysis.
8. Tubes to prepare standard or sample dilutions.
9. Heating block or water bath capable of 80°C


#### V. REAGENT PREPARATION

1. Bring wash buffer, samples, assay diluents, and PCR plate to room temperature (18 - 25 °C) before use. PCR master mix (Item J) and Primer solution (Item I) should be kept at 4 °C at all times.
2. Sample dilution: If your samples need to be diluted, 1x Assay Diluent B (Item E) should be used for dilution of serum/plasma samples. Assay Diluent A maybe used in place if significant matrix affects are seen.  
Suggested dilution for normal serum/plasma: 2 - 10 fold\*.

\*Please note that levels of the target protein may vary between different specimens. Optimal dilution factors for each sample must be determined by the investigator.

3. Assay Diluent B should be diluted 5-fold with deionized water.
4. Briefly spin the Detection Antibody vial (Item F) before use. Add 25 µl of 1X Assay Diluent (Item D) into the vial to prepare a detection antibody concentrate. Pipette up and down to mix gently (the concentrate can be stored at 4 °C for 5 days). This concentrate should be diluted 80-fold with 1X Assay Diluent (Item D) and used in step 4 of the Assay Procedure.
5. PCR preparation buffer (Item K) should be transferred to a 15mL tube and diluted with 9mL of deionized or distilled water before use.
6. Final Wash Buffer (Item L) should be transferred to a 15mL tube and diluted with 9mL of deionized or distilled water for every 1mL of 10x concentrate used before use.
7. Preparation of standard: Add 400 µl Assay Diluent A (Item D) to the vial to prepare a 50 ng/ml standard. Dissolve the powder thoroughly by gentle mixing. Add 120 µl TNFa standard from the vial of Item C, into a tube with 880 µl Assay Diluent A to prepare a 6000 pg/ml standard solution. Use the 6000 pg/ml standard solution to produce a

dilution series (shown below) by pipetting 300µl of Assay Diluent A into each tube and transferring 100µL for the previous standard into the new tube. Mix each tube thoroughly before the next transfer. Assay Diluent A or 1x Assay Diluent B serves as the zero standard (0 pg/ml).

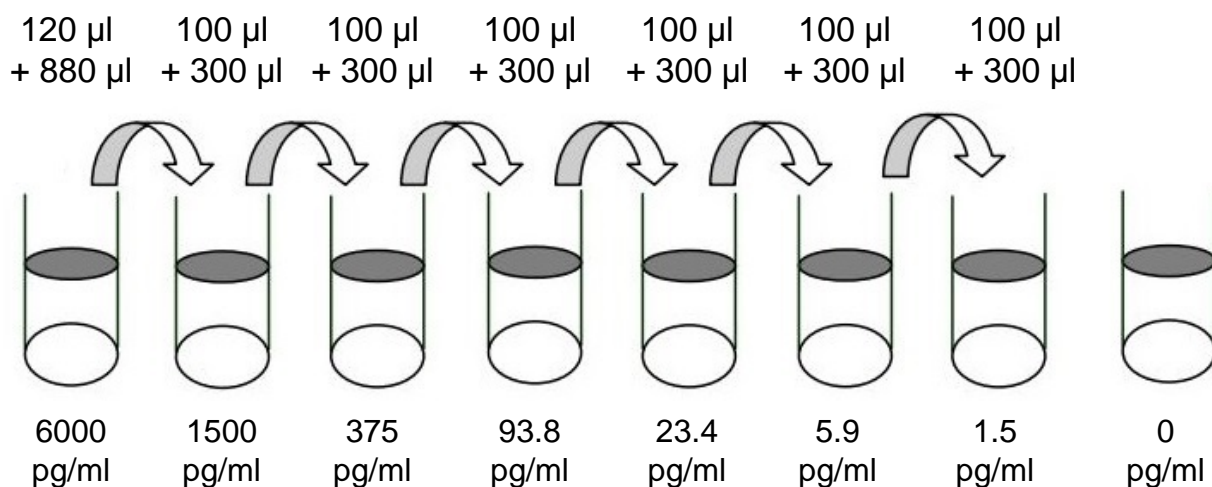

8. If the Wash Buffer Concentrate (20x) (Item B) contains visible crystals, warm to room temperature and mix gently until dissolved. Dilute 20 ml of Wash Buffer Concentrate into deionized or distilled water to yield 400 ml of 1x Wash Buffer.
9. Prepare the IQELISA detection reagent by calculating how much will be needed. This may be accomplished by multiplying the number of wells to be assayed by the volume you plan to use per well. Once the volume of IQELISA detection reagent is known, prepare the reagent by diluting it 1:10 with deionized water and mixing thoroughly.


## VI. ASSAY PROCEDURE

1. Bring all reagents and samples to room temperature (18 - 25°C) before use. It is recommended that all standards and samples be run in triplicate. The plate may be broken into strips so that you only use the amount you need, and the rest can be saved for use at a later date.
2. Add 10-25µl of each standard (see Reagent Preparation step 2) and sample into appropriate wells. Volumes should be consistent between all wells, samples, and standards. As little as 10µL can be used if sample volume is limited, however this increases the chance of technical error. Ensure there are no bubbles present at the bottom of the wells. Dislodge any bubbles with gentle tapping or with a pipette tip being careful not to contact the sides or bottom of the well. Cover well and incubate for 2.5 hours at room temperature or overnight at 4°C with gentle shaking.
3. Discard the solution and wash 4 times with 1x Wash Solution. Wash by filling each well with Wash Buffer (100 µl) using a multi-channel Pipette or autowasher. Complete

removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.

4. Add 25 µl of prepared Detection Antibody (Reagent Preparation step 4) to each well. Incubate for 1 hour at room temperature with gentle shaking.
5. Discard the solution. Repeat the wash as in step 3.
6. Add 25µL of prepared IQELISA detection reagent and incubate 1 hour with rocking (Item G Reagent Preparation step 9)
7. Discard the solution. Repeat the wash as in step 3.
8. Add 100µL of Final wash buffer (Item L) to each well and incubate for 5 minutes with rocking. Remove the solution from each well and repeat an additional 2x.
9. Add 100µL of 1x PCR preparation buffer (Item K) to each well and incubate with rocking for 5 minutes before removing the buffer. Blot the plate after the buffer is removed to ensure complete removal of the buffer.
10. Add 15µL of the Primer solution (Item I) to each well of the plate. At this stage the plate can be covered and stored at -20 °C for use the next day if needed.
11. Add 10µL of PCR Master Mix (Item J) to each well and pipette thoroughly to mix the well (at least 3x up and down).
12. Cover the plate with the supplied caps taking care to press firmly on each well, ensuring that tubes are completely closed. It may be helpful to remove each strip from the others and cap individually.

13. Place the plate into a real-time PCR instrument using a FITC compatible wave length for detection with the following settings for cycling
  1. 3 minute activation at 95°C
  2. 10 seconds 95°C denaturation
  3. 25 seconds 55°C annealing/extension
  4. Repeat steps 2 and 3 29x

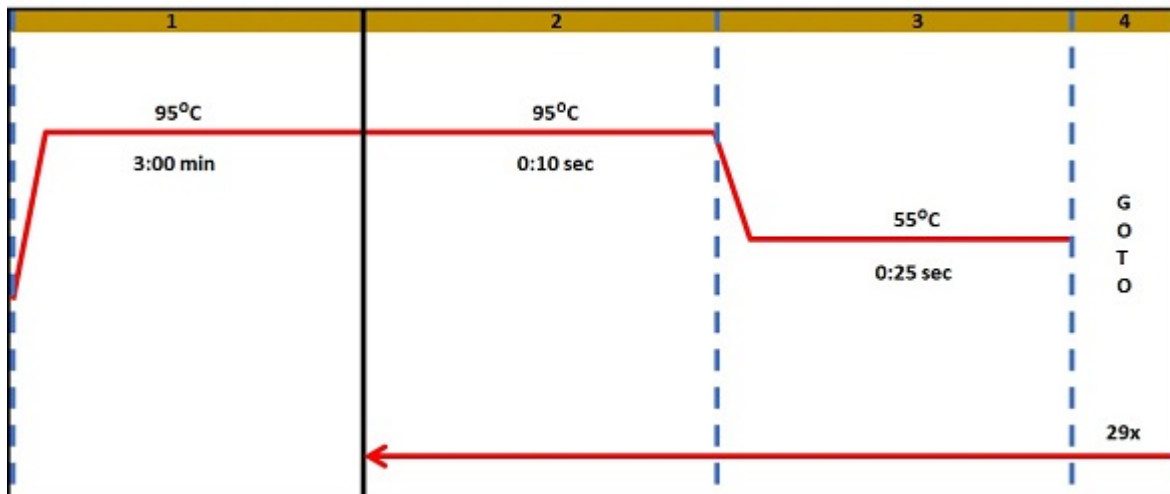

## VII. ASSAY PROCEDURE SUMMARY

1. Prepare all reagents, samples and standards as instructed.
2. Add 25µl standard or sample to each well.  
Incubate 2.5 hours at room temperature or overnight at 4°C.
3. Add 25µl Detection Antibody to each well.  
Incubate 1 hour at room temperature.
4. Add 25µL of IQELISA Detection Reagent to each well. Incubate 1 hour
5. Add 15µl Primer solution and 10µL of PCR master mix to each well
6. Run real-time PCR

## VIII. CALCULATION OF RESULTS

The primary data output of the IQELISA kit is  $C_t$  values. These values represent the number of cycles required for a sample to pass a fluorescence threshold. As the DNA is amplified additional fluorescent signal is produced, with each cycle resulting in an approximate doubling of the DNA. Therefore, higher levels of DNA (directly related to the amount of antigen in the sample) result in lower  $C_t$  values.

Calculate the mean  $C_t$  for each set of triplicate standards, controls and samples. Subtract the  $C_t$  value of each sample from the control to obtain the difference between the control and sample (Delta  $C_t$ ). Plot the values of the standards on a graph using a log scale for concentration on the x axis. This graph is the quickest way to visualize results, although not the most accurate. If this method is used the concentration of unknown samples can be estimated using a logarithmic line of best fit.

The line of best fit will have an equation  $y = m\ln(x)+b$ , where y is the Delta  $C_t$  value and x is the concentration. It may be helpful to use 5 significant figures for m and b to minimize rounding errors. To calculate the concentration of unknown sample this can be entered into Excel in the following format

`=EXP((y-b)/m))`


Where y is the Delta  $C_t$  obtained during the assay, and b and m are obtained from the line of best fit

Alternatively, for a more accurate representation linear regression may be used. Both the Delta  $C_t$  and Concentration can be transformed using a log base of 10, plotted on a graph as described above, along with a line of best fit (using a linear model). The equation of this line may be used to calculate the antigen concentration of unknown samples. This is the method used for the analysis spreadsheet for IQELISA available online.



## A. TYPICAL DATA

These data are for demonstration only. A standard curve must be run with each assay.

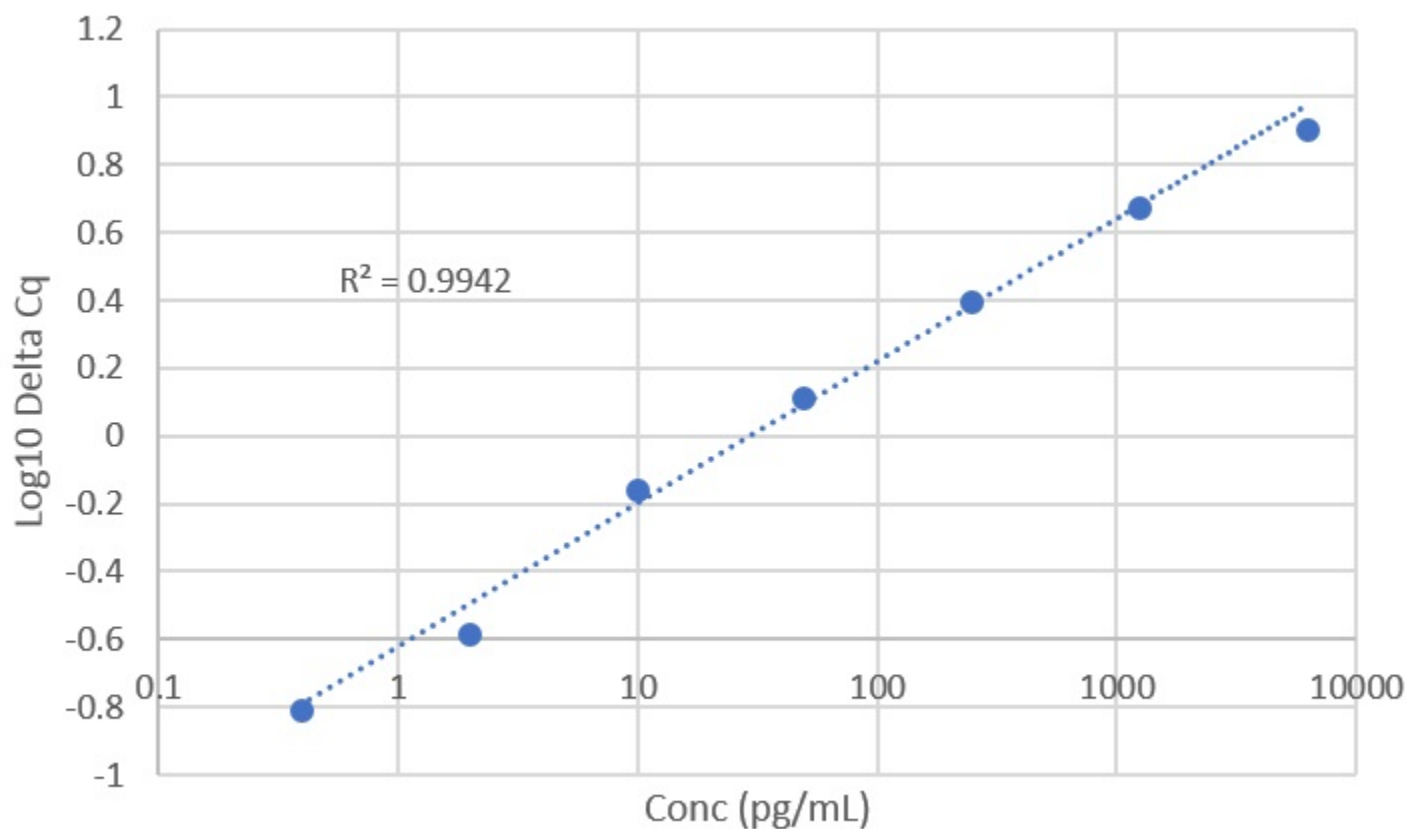

## B. SENSITIVITY and RECOVERY

The minimum quantifiable dose of TNFa is typically 10 pg/ml, however levels as low as 10 pg/ml may be detected outside of the quantification range.

Serum spike tests show recovery is 131% with a range of 141% to 119%

Intraplate CV is below 10% for all samples and Interplate CV is below 15%

## X. TROUBLESHOOTING GUIDE

| Problem             | Cause                                                                                                                                                    | Solution                                                                                                                                                                                                                                           |
|---------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Poor standard curve | <ul style="list-style-type: none"> <li>• Inaccurate pipetting</li> <li>• Improper standard dilution</li> </ul>                                           | <ul style="list-style-type: none"> <li>• Check pipettes</li> <li>• Briefly centrifuge Item C and dissolve the powder thoroughly by gently mixing</li> </ul>                                                                                        |
| Low signal          | <ul style="list-style-type: none"> <li>• Too brief incubation times</li> <li>• Inadequate reagent volumes or improper dilution</li> </ul>                | <ul style="list-style-type: none"> <li>• Ensure sufficient incubation time. Assay procedure step 2 may be done overnight</li> <li>• Check pipettes and ensure correct preparation</li> </ul>                                                       |
| Large CV            | <ul style="list-style-type: none"> <li>• Uneven pipetting</li> <li>• Bubbles present in wells</li> </ul>                                                 | <ul style="list-style-type: none"> <li>• Check pipettes</li> <li>• Lightly tap or use pipette tip to dislodge from bottom of well</li> </ul>                                                                                                       |
| High background     | <ul style="list-style-type: none"> <li>• Plate is insufficiently washed</li> <li>• Contaminated wash buffer</li> <li>• Improper T<sub>m</sub></li> </ul> | <ul style="list-style-type: none"> <li>• Review the manual for proper wash. If using a plate washer, ensure that all ports are unobstructed.</li> <li>• Make fresh wash buffer</li> <li>• Check run parameters and calibrate instrument</li> </ul> |
| Low sensitivity     | <ul style="list-style-type: none"> <li>• Improper storage of the IQELISA kit</li> <li>• Improper T<sub>m</sub></li> </ul>                                | <ul style="list-style-type: none"> <li>• Store your standard at &lt;-20°C after reconstitution, others at 4°C.</li> <li>• Check run parameters and calibrate instrument</li> </ul>                                                                 |

This product is for research use only.



©2019 RayBiotech, Inc