

# Medical Product Guide

The global leader in health monitoring

## Vision:

We aim to create a society where people around the world can expand their potential through health habits and feel happy.

## Mission:

We will continue to create health standards in various fields from a new perspective.



Until now, Tanita has been working on the development and sale of measuring instruments that “measure health” with the philosophy of contributing to the health promotion of people around the world through “measurement.” In addition to this, the women’s fitness “Fitzmee” was opened in 2004, and the “Marunouchi Tanita Shokudo” was opened in 2012. In 2014, we started offering the Tanita Health Program, a group health promotion package for companies and local governments, and are expanding our business to include health promotion services.

Today is said to be the “100 years of life”. The time has come when extending healthy life expectancy is important for both individuals and society. From now on, Tanita will work to create a society where people around the world can feel happiness through health promotion.

**May everyone live their own way and spend precious time with those around them. Tanita will support the continuation of “Healthy Habits” for that purpose.**

株式会社 タニタ 谷田 千里  
代表取締役社長

Mr Tanida san

TANITA; established in 1944 with its global headquarters in Tokyo, has become known as the global market leader in precision scales and body composition monitors, with over 100 million devices sold worldwide.

As an innovator in the field of Bioelectrical Impedance Analysis (BIA), TANITA is recognized as the GOLD standard in the industry, based on extensive validation studies behind its 4C technology and superb product quality, which we proudly back-up with an unparalleled guarantee period.

Recently, TANITA has introduced an appealing new company mission; 'Healthy Habits for Happiness' which demonstrates our ambition to not only Measure and Monitor health, but also to Motivate people towards creating and maintaining a healthy lifestyle step by step.

Recent studies\* have shown that monitoring one's progress against a goal increases the likelihood of attaining the goal by up to 80%. TANITA prides itself in being the only supplier of BIA devices for professional use, that also offers BIA technology in body composition scales for home use, offering everyone the opportunity to monitor their progress on a regular basis.

After the launch of TANITA restaurants in Japan; where you can select your healthy meal up to a maximum of 500kcal, TANITA Europe now introduces its new TANITA branded Clever Coffee concept, which increases metabolism through high levels of the natural ingredient chlorogenic acid. A first new initiative in Europe supporting our mission to help people improve their holistic health and wellbeing!

*Jan Alderlieste,*  
**CEO TANITA Europe B.V.**



\* Benjamin Harkin, Thomas L. Webb, and Betty P. I. Chang, Andrew Prestwich, Mark Conner, Ian Kellar, Yael Benn, Paschal Sheeran. **Does Monitoring Goal Progress Promote Goal Attainment? A Meta-Analysis of the Experimental Evidence.** Psychological Bulletin, American Psychological Association, 2016, Vol. 142, No. 2, 198 -229









**WORLD No.1  
BIA BRAND**

**UNPARALLELED  
GUARANTEE**



# Why Tanita Bioelectrical Impedance Analysis technology is the most accurate

## Highest levels of precision and clinical accuracy.

The original prediction equations used in Tanita software were devised by world-renowned body composition expert Professor Steven Heymsfield and his research team at St Luke's Roosevelt Hospital, Columbia University, New York. Extensive independent research has proven that the accurate prediction of an individual's body composition can only be determined if a range of parameters are included in an algorithm, such as gender, age and height and weight.

## Trusted by experts for clinical excellence.

Tanita BIA technology has been more extensively validated against alternative body composition techniques than any other company and the findings have been published in international medical journals. In addition, Tanita monitors have been used in hundreds of independent research studies worldwide. Tanita is regarded by the scientific community as the gold standard in BIA technology and the Tanita Medical Advisory Board ensures Tanita remains at the forefront of scientific advances. For more information on our extensive scientific publications and validation visit: <https://tanita.eu/tanita-academy/for-professionals/the-science>

## Ground breaking advances in research.

Tanita continually invests in numerous research projects that focus on enhancing understanding of key health and fitness issues, including areas such as childhood obesity, optimising physical performance and sarcopenia in the elderly. Our

aim is to work with experts to develop tools and technologies to assist all healthcare and sports professionals in providing the best possible services and to help people enjoy healthier lives.

## Repeatability of measurements through precision weighing.

Precise weight measurements are essential for calculating accurate body composition measurements. Tanita prides itself on manufacturing highly accurate weighing mechanisms in both its home use and professional models. All Tanita medically approved professional monitors have been awarded NAWI Certification as well MDD Class IIa, FDA and CE Approval ensuring the highest standards are met.

## Sound quality through robust construction.

Tanita has grown through continuous product innovation and a commitment to maintaining the highest manufacturing quality standards. The company operates award-winning manufacturing facilities in Japan and China and all Tanita medical products meet strict international quality standards and are independently quality-controlled.

**M**

The scales with this symbol are validated to be accurate and legal for use within the medical sector according to EU regulations. It is compulsory to use a product with this compliance for use in all medical settings.



The scales with this symbol have been calibrated according to the precision class III in the Directive 2009 / 23 /EC





# MAKING A DIFFERENCE

TO OUR PATIENTS' LIVES  
THANKS TO USING  
THE BEST TECHNOLOGY


“ As a Medical Advisory Board member, I have consulted with and learned from Tanita engineers for over 20 years as they developed early prototypes that have now blossomed into advanced bioimpedance technologies that accurately quantify body composition.

These developments are timely as a critical need exists to go beyond simple but inaccurate measures of body shape and composition (e.g., body mass index) when evaluating people with obesity, sarcopenia, and other chronic medical conditions and diseases. ”

## Professor Steven Heymsfield

Executive Director of Pennington Biomedical  
Research Center, Baton Rouge USA.

**Member of Tanita Medical Advisory Board**

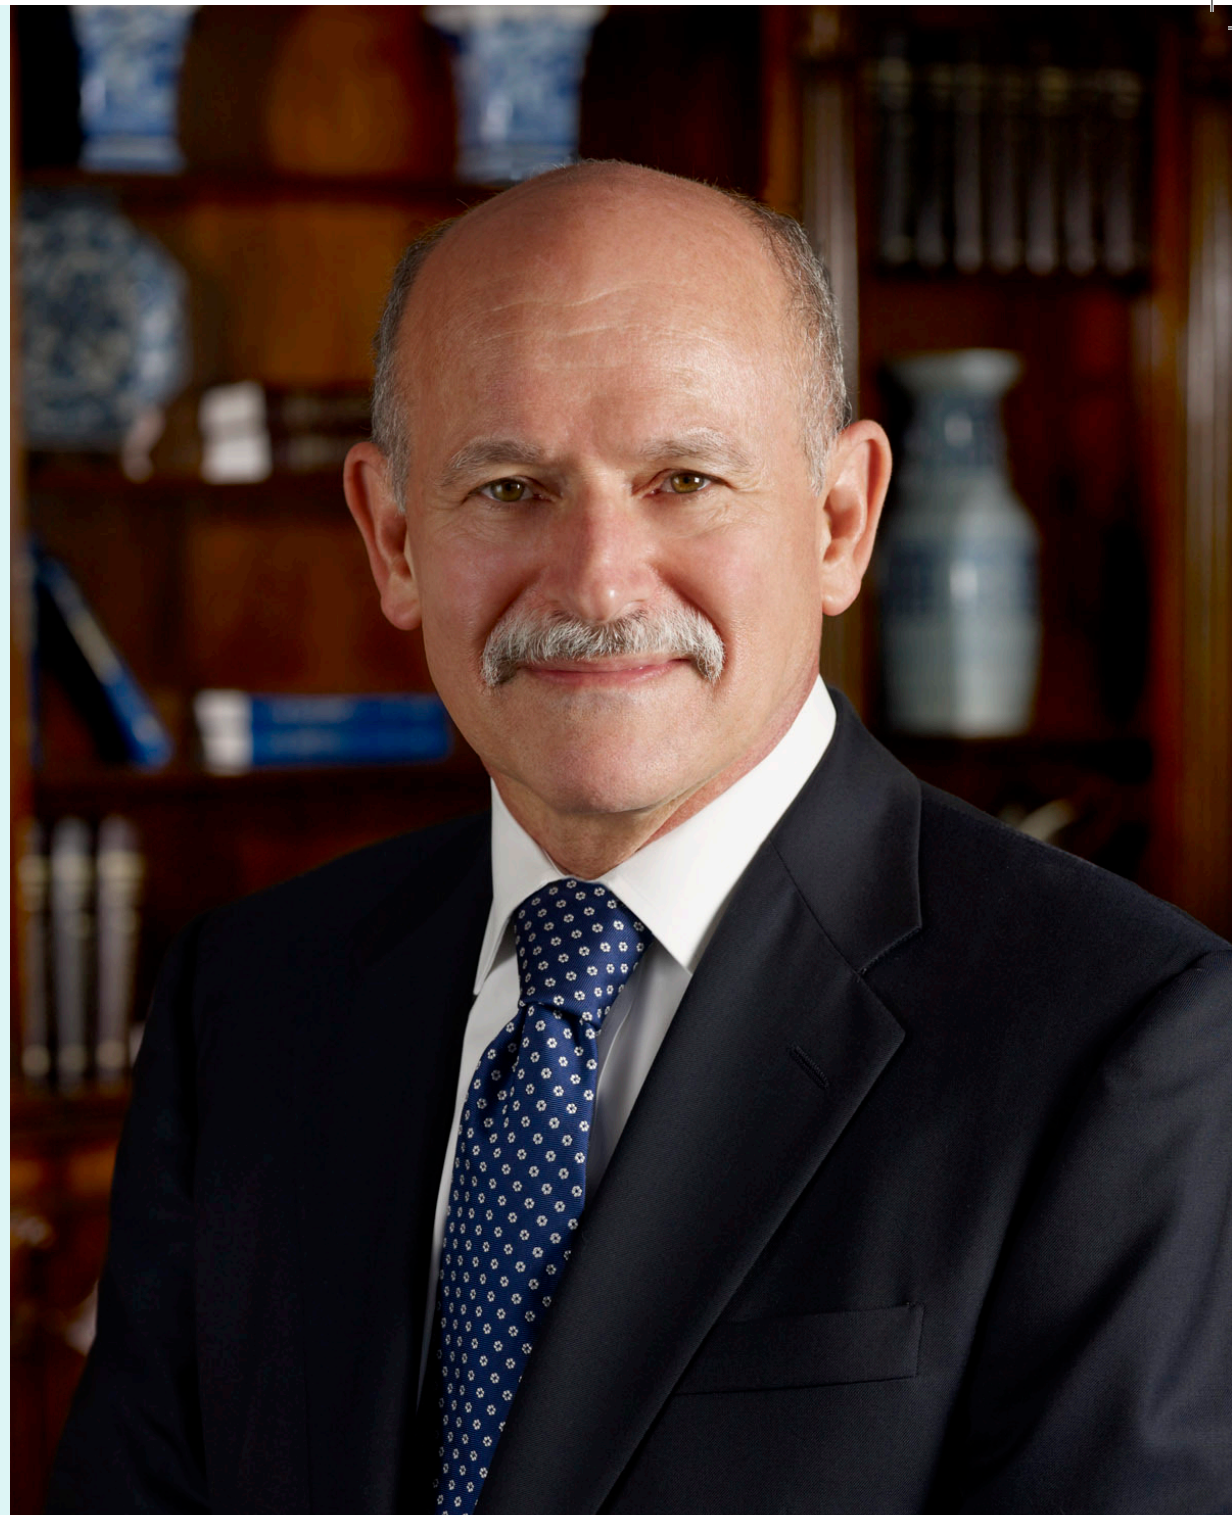



# Welcome to the next level in **4c**curacy

## Introducing the 4-Compartment measurement from Tanita

Tanita continues to offer the most accurate calculation of fat, lean mass (or muscle) and bone mineral density available, but with 4C monitoring we go even further, giving an unparalleled, 4-Compartment measurement.

Our new 4C method will enable you to fully assess levels of body fat, protein, bone mineral mass and water within the body.

## What is the 4-Compartment (4C) model?

The 4C model divides body weight into fat, water, mineral, and protein using the gold standard method for measuring each element.

The 4C model involves the measurement of body mass or weight, total body volume (air displacement), total body water (D2O), and bone mineral (DXA); however, specialized laboratory equipment is required minimizing the availability of the 4C method to many clinicians and researchers.

**Fat mass**

**97%**

accuracy as compared with the 4C method<sup>(1)</sup>

**Fat free mass**

**98%**

accuracy as compared with the 4C method<sup>(1)</sup>

**Muscle mass**

**98%**

accuracy as compared with the 4C method<sup>(1)</sup>

**Total body water**

**98%**

accuracy as compared with the 4C method (D2O)<sup>(1)</sup>

<sup>(1)</sup>Nishizawa, M & Ikeda, Y (2018) 'Effectiveness of measuring body composition and metabolism in diet', Metabolic Sensing - Learn the Metabolism in Health, Dieting, Beauty, Medicine and Brain. CMC Publishing Co., Chapter 6, Page 49



*"The 4-Compartment model is a gold standard method to assess body composition in many conditions such as over and under nutrition, hydration, obesity and sarcopenia."*

## **Angelo Pietrobelli, M.D.**

Professor of Pediatrics  
Professor of Nutrition  
Pediatric Unit

Department of Surgical Sciences,  
Dentistry, Gynecology and Pediatrics,  
University of Verona, Verona, Italy

**Member of Tanita Medical  
Advisory Board**

# Validation

National and international regulatory standards continue to evolve and become more stringent. Medical devices are also becoming smaller and more complex in design, using advanced, engineered materials. This makes the process of validation and verification even more important—not only to comply with regulations, but also design the highest-quality part and production process. The result is better repeatability, fewer mistakes, less rework and redesign, faster time to market, improved competitiveness, and lower costs.

Validation is the process of making sure that you have objective evidence that user needs and intended uses are met. It is usually done by tests, inspections, and in some cases analysis. However, the target of the validation is to make sure the user needs are met in a medical device that consistently provides the intended medical benefit in actual-use conditions. Verification is typically making sure that you have objective evidence that specified requirements are met. It is usually done by tests, inspections, and in some cases analysis as well.

## Tanita's professional body composition monitors have been validated.

Validation papers are available on request.

### Sarcopenic obesity: clinical diagnostic potential of 8-electrode multi-segment BIA

Jolene Zheng, Bin Zhu, Chenfei Gao, James Matthew Watson, Lina Sallou, Guang Jia, Steven B. Heymsfield, Pennington Biomedical Research Center, Department of Physics and Astronomy, Louisiana State Univ. System, Baton Rouge, LA

#### Introduction

Sarcopenic obesity, a pathological state with excess fat and depleted skeletal muscle mass (SM), is increasingly being recognized as a phenotype associated with adverse clinical outcomes.

#### STUDY AIMS

To answer the question: how does 8-electrode multi-segment bioimpedance analysis (BIA; MC780 and MC980) compare to dual-energy x-ray absorptiometry (DXA) as the reference for estimating SM? Similarly, how well do the BIA systems associate with fat mass measured using 4-component reference methods?

#### Methods

**Appendicular lean soft tissue (LST)**, a measure of SM; arm, leg, and total, was measured by DXA (GE, DXA) and compared to predicted SM by the two BIA systems (MC780 and MC980) (Tanita Corp., Tokyo, Japan) in 130 healthy men and women age  $\geq 18$  yrs varying in BMI.

**Body fat** measured with multi-component models (Wang [Wang and Lohman 1981]) as the reference were compared to BIA results. 4-component models: body volume by Bod Pod; total body water by deuterium dilution; and bone mineral mass by DXA.

Both BIA systems are based on an 8-electrode configuration that separately captures each arm and leg along with trunk and right and left-body electrical properties.

#### Results

**Subject Characteristics.** 68 F, 62 M; 4 Asian, 27 African American, 97 Caucasian, 2 Other. Age: 52.2  $\pm$  9.3 yrs. Height: 167.6  $\pm$  13.5 cm. Weight: 78.9  $\pm$  22.8 kg.

The MC780 and 980 results were similar for all measures: Leg, arm, and total limb fat mass and LST for DXA and limb fat and SM mass by BIA (MC980; kg, Xs SD). (See Table 1 for details.)

|       | Leg  | Arm  | Total |
|-------|------|------|-------|
| MC780 | 0.94 | 0.94 | 0.94  |
| MC980 | 0.94 | 0.94 | 0.94  |
| DXA   | 0.94 | 0.94 | 0.94  |

Figure 2. Tanita MC980. The line of identity is shown in the figure.

Figure 3. Tanita MC980. The line of identity is shown in the figure.

Figure 4. Tanita MC980. The line of identity is shown in the figure.

\*Correlations (r-values) between component models. Bod Pod, are shown in the table; all are correlated. A BIA example is shown in Figure 1.

Figure 1. Tanita MC980. The line of identity is shown in the figure.

Figure 2. Tanita MC980. The line of identity is shown in the figure.

Figure 3. Tanita MC980. The line of identity is shown in the figure.

Figure 4. Tanita MC980. The line of identity is shown in the figure.

Figure 5. Tanita MC980. The line of identity is shown in the figure.

Figure 6. Tanita MC980. The line of identity is shown in the figure.

Figure 7. Tanita MC980. The line of identity is shown in the figure.

Figure 8. Tanita MC980. The line of identity is shown in the figure.

Figure 9. Tanita MC980. The line of identity is shown in the figure.

Figure 10. Tanita MC980. The line of identity is shown in the figure.

Figure 11. Tanita MC980. The line of identity is shown in the figure.

Figure 12. Tanita MC980. The line of identity is shown in the figure.

Figure 13. Tanita MC980. The line of identity is shown in the figure.

Figure 14. Tanita MC980. The line of identity is shown in the figure.

Figure 15. Tanita MC980. The line of identity is shown in the figure.

### Sarcopenic obesity: clinical diagnostic potential of 8-electrode multi-segment BIA

Angelo Pietroboli, Callie Johnson, Steven B. Heymsfield, Jolene Zheng, Pennington Biomedical Research Center, Louisiana State Univ. System, Baton Rouge, LA, USA; University of Virginia, Charlottesville, VA, USA

#### Abstract

**Background:** Phase angle (PA), derived from bioelectrical impedance analysis (BIA), is a measure of cellular health and is associated with changes in cellular water content. PA is a measure of cellular health and is associated with changes in cellular water content. PA is a measure of cellular health and is associated with changes in cellular water content.

**Results:** Significant correlations (p < 0.05) were present for leg, arm, and total limb fat mass and LST for DXA and limb fat and SM mass by BIA (MC980; kg, Xs SD). (See Table 1 for details.)

**Conclusions:** Measurement of PA may be a simple, practical, and clinically useful measure of age-related changes in SM quality that can be studied in the context of sarcopenic obesity and related clinical outcomes.

**Objectives:** Sarcopenic obesity, a pathological state with excess fat and depleted skeletal muscle mass (SM), is increasingly being recognized as a phenotype associated with adverse clinical outcomes.

**STUDY AIMS:** To answer the question: how does 8-electrode multi-segment bioimpedance analysis (BIA; MC780 and MC980) compare to dual-energy x-ray absorptiometry (DXA) as the reference for estimating SM? Similarly, how well do the BIA systems associate with fat mass measured using 4-component reference methods?

**Methods:** **Appendicular lean soft tissue (LST)**, a measure of SM; arm, leg, and total, was measured by DXA (GE, DXA) and compared to predicted SM by the two BIA systems (MC780 and MC980) (Tanita Corp., Tokyo, Japan) in 130 healthy men and women age  $\geq 18$  yrs varying in BMI.

**Body fat** measured with multi-component models (Wang [Wang and Lohman 1981]) as the reference were compared to BIA results. 4-component models: body volume by Bod Pod; total body water by deuterium dilution; and bone mineral mass by DXA.

Both BIA systems are based on an 8-electrode configuration that separately captures each arm and leg along with trunk and right and left-body electrical properties.

Figure 1. Tanita MC980. The line of identity is shown in the figure.

Figure 2. Tanita MC980. The line of identity is shown in the figure.

Figure 3. Tanita MC980. The line of identity is shown in the figure.

Figure 4. Tanita MC980. The line of identity is shown in the figure.

Figure 5. Tanita MC980. The line of identity is shown in the figure.

Figure 6. Tanita MC980. The line of identity is shown in the figure.

Figure 7. Tanita MC980. The line of identity is shown in the figure.

Figure 8. Tanita MC980. The line of identity is shown in the figure.

Figure 9. Tanita MC980. The line of identity is shown in the figure.

Figure 10. Tanita MC980. The line of identity is shown in the figure.

Figure 11. Tanita MC980. The line of identity is shown in the figure.

Figure 12. Tanita MC980. The line of identity is shown in the figure.

Figure 13. Tanita MC980. The line of identity is shown in the figure.

Figure 14. Tanita MC980. The line of identity is shown in the figure.

Figure 15. Tanita MC980. The line of identity is shown in the figure.

Figure 16. Tanita MC980. The line of identity is shown in the figure.

Figure 17. Tanita MC980. The line of identity is shown in the figure.

#### Conclusion

\*8-electrode multi-segment BIA has the potential for diagnosing sarcopenic obesity in the clinical setting.

Figure 1. Tanita MC980. The line of identity is shown in the figure.

Figure 2. Tanita MC980. The line of identity is shown in the figure.

Figure 3. Tanita MC980. The line of identity is shown in the figure.

Figure 4. Tanita MC980. The line of identity is shown in the figure.

Figure 5. Tanita MC980. The line of identity is shown in the figure.

Figure 6. Tanita MC980. The line of identity is shown in the figure.

Figure 7. Tanita MC980. The line of identity is shown in the figure.

Figure 8. Tanita MC980. The line of identity is shown in the figure.

### Sarcopenic obesity: clinical diagnostic potential of 8 - electrode multi - segment BIA

### Skeletal Muscle Quality: Concordant Findings from Two Practical Non-Invasive Approaches

Angelo Pietroboli, Callie Johnson, Steven B. Heymsfield, Jolene Zheng, Pennington Biomedical Research Center, Louisiana State Univ. System, Baton Rouge, LA, USA

#### Abstract

**Background:** Phase angle (PA), derived from bioelectrical impedance analysis (BIA), is a measure of cellular health and is associated with changes in cellular water content. PA is a measure of cellular health and is associated with changes in cellular water content. PA is a measure of cellular health and is associated with changes in cellular water content.

**Results:** Significant correlations (p < 0.05) were present for leg, arm, and total limb fat mass and LST for DXA and limb fat and SM mass by BIA (MC980; kg, Xs SD). (See Table 1 for details.)

**Conclusions:** Measurement of PA may be a simple, practical, and clinically useful measure of age-related changes in SM quality that can be studied in the context of sarcopenic obesity and related clinical outcomes.

**Objectives:** Sarcopenic obesity, a pathological state with excess fat and depleted skeletal muscle mass (SM), is increasingly being recognized as a phenotype associated with adverse clinical outcomes.

**STUDY AIMS:** To answer the question: how does 8-electrode multi-segment bioimpedance analysis (BIA; MC780 and MC980) compare to dual-energy x-ray absorptiometry (DXA) as the reference for estimating SM? Similarly, how well do the BIA systems associate with fat mass measured using 4-component reference methods?

**Methods:** **Appendicular lean soft tissue (LST)**, a measure of SM; arm, leg, and total, was measured by DXA (GE, DXA) and compared to predicted SM by the two BIA systems (MC780 and MC980) (Tanita Corp., Tokyo, Japan) in 130 healthy men and women age  $\geq 18$  yrs varying in BMI.

**Body fat** measured with multi-component models (Wang [Wang and Lohman 1981]) as the reference were compared to BIA results. 4-component models: body volume by Bod Pod; total body water by deuterium dilution; and bone mineral mass by DXA.

Both BIA systems are based on an 8-electrode configuration that separately captures each arm and leg along with trunk and right and left-body electrical properties.

Figure 1. Tanita MC980. The line of identity is shown in the figure.

Figure 2. Tanita MC980. The line of identity is shown in the figure.

Figure 3. Tanita MC980. The line of identity is shown in the figure.

Figure 4. Tanita MC980. The line of identity is shown in the figure.

Figure 5. Tanita MC980. The line of identity is shown in the figure.

Figure 6. Tanita MC980. The line of identity is shown in the figure.

Figure 7. Tanita MC980. The line of identity is shown in the figure.

Figure 8. Tanita MC980. The line of identity is shown in the figure.

Figure 9. Tanita MC980. The line of identity is shown in the figure.

Figure 10. Tanita MC980. The line of identity is shown in the figure.

Figure 11. Tanita MC980. The line of identity is shown in the figure.

Figure 12. Tanita MC980. The line of identity is shown in the figure.

Figure 13. Tanita MC980. The line of identity is shown in the figure.

Figure 14. Tanita MC980. The line of identity is shown in the figure.

Figure 15. Tanita MC980. The line of identity is shown in the figure.

Figure 16. Tanita MC980. The line of identity is shown in the figure.

Figure 17. Tanita MC980. The line of identity is shown in the figure.

Figure 18. Tanita MC980. The line of identity is shown in the figure.

Figure 19. Tanita MC980. The line of identity is shown in the figure.

Figure 20. Tanita MC980. The line of identity is shown in the figure.

Figure 21. Tanita MC980. The line of identity is shown in the figure.

Figure 22. Tanita MC980. The line of identity is shown in the figure.

Figure 23. Tanita MC980. The line of identity is shown in the figure.

Figure 24. Tanita MC980. The line of identity is shown in the figure.

#### Conclusion

\*8-electrode multi-segment BIA has the potential for diagnosing sarcopenic obesity in the clinical setting.

Figure 1. Tanita MC980. The line of identity is shown in the figure.

Figure 2. Tanita MC980. The line of identity is shown in the figure.

Figure 3. Tanita MC980. The line of identity is shown in the figure.

Figure 4. Tanita MC980. The line of identity is shown in the figure.

Figure 5. Tanita MC980. The line of identity is shown in the figure.

Figure 6. Tanita MC980. The line of identity is shown in the figure.

Figure 7. Tanita MC980. The line of identity is shown in the figure.

Figure 8. Tanita MC980. The line of identity is shown in the figure.

Figure 9. Tanita MC980. The line of identity is shown in the figure.

Figure 10. Tanita MC980. The line of identity is shown in the figure.

Figure 11. Tanita MC980. The line of identity is shown in the figure.

Figure 12. Tanita MC980. The line of identity is shown in the figure.

Figure 13. Tanita MC980. The line of identity is shown in the figure.

### Skeletal Muscle Quality: Concordant Findings from Two Practical Non-Invasive Approaches

# Validation studies

## Tanita BIA technology: A scientific overview of methods and accuracy

Tanita BIA technology was first introduced in 1992. Since then we have strived to establish the most accurate technology and will always look for ways and methods to improve accuracy through dedicated research and development.

The Tanita algorithm is the cornerstone of precision body composition measurements in different body types, ages and gender. This has been repeatedly shown in independent scientific publications from researchers and clinicians worldwide.

There are various parameters within the algorithm to ensure the highest accuracy. These include AGE, GENDER and ETHNICITY. By incorporating these parameters, Tanita BIA technology can provide more consistent and reliable body composition measurements for anyone who steps on.

These factors are incorporated into most BIA technology manufacturers within the medical and research fields and has proven to be the foundation of strong validation. This is shown in scientific publications and highlights the importance of including AGE, GENDER and ETHNICITY when calculating body composition of individuals.

In addition, Tanita has developed algorithms for adults with a higher level of physical activity – athlete mode. This feature allows higher accuracy of assessing individuals muscle mass.

## Recent publications showing the importance of incorporating the different parameters in the scientific literature:

### AGE and GENDER

The following papers highlight the importance of incorporating age and gender into BIA technology algorithms and the impact on accuracy when they are not included:

- Völgyi E, Tylavsky FA, Lyytikäinen A, Suominen H, Alén M, Cheng S. **Assessing body composition with DXA and bioimpedance: effects of obesity, physical activity, and age.** Obesity 2008;16(3):700-5.

**Conclusion:** Compared to DXA, both BIA devices provided on average 2-6% lower values for FM% in normal BMI men, in women in all BMI categories, and in both genders in both HPA and LPA groups. In obese men, the differences were smaller. The two BIA devices provided similar means for groups. **Differences between the two BIA devices with increasing FM% were a result of the InBody (720) not including age in their algorithm for estimating body composition.**

- Faria SL, Faria OP, Cardeal MD, Ito MK. **Validation study of multi-frequency bioelectrical impedance with dual-energy X-ray absorptiometry among obese patients.** Obes Surg 2014; 24(9):1476-80.

**Conclusion:** BIA proved to be a safe alternative for assessing BC in clinically severely obese patients and thus provides a more accessible evaluation tool for this population. **But, consideration should be given to the formula added to the BIA measurement, adjusting the values to differences observed in order to reduce errors when compared with the DXA measurements**



- Völgyi E, Tylavsky FA, Lyytikäinen A, Suominen H, Alén M, Cheng S. **Assessing body composition with DXA and bioimpedance: effects of obesity, physical activity, and age.** Obesity 2008; 16(3):700-5.

**Conclusion:** Compared to DXA, both BIA devices (Tanita MC180 and Inbody 720) provided on average 2-6% lower values for FM% in normal BMI men, in women in all BMI categories, and in both genders in both HPA and LPA groups. In obese men, the differences were smaller. The two BIA devices provided similar means for groups. **Differences between the two BIA devices with increasing FM% were a result of the InBody (720) not including age in their algorithm for estimating body composition**

- Karelis AD, Chamberland G, Aubertin-Leheudre M, Duval C; Ecological mobility in Aging and Parkinson (EMAP) group. **Validation of a portable bioelectrical impedance analyzer for the assessment of body composition.** Appl Physiol Nutr Metab. 2013 Jan;38(1):27-32.

**Conclusion:** the present study indicated that the portable Inbody 230 may be an acceptable device to measure fat mass, % body fat, and total FFM (except for women) in healthy adults. **In addition, there appears to be a systematic bias for the estimation of trunk and appendicular FFM with the Inbody 230 in men and women.**

- Sillanpää E, Cheng S, Häkkinen K, Finni T, Walker S, Pesola A, Ahtiainen J, Stenroth L, Selänne H, Sipilä S. **Body composition in 18- to 88-year-old adults--comparison of multifrequency bioimpedance and dual-energy X-ray absorptiometry.** Obesity 2014; 22(1):101-9

**Authors note:** "we also found that age was a significant predictor in all body composition estimates both in women and in men. Although age and sex are often employed in BIA algorithms because of an increase in measurement accuracy".



## ETHNICITY and GENDER

The following papers conclude Ethnicity increases accuracy of adult and children's body composition measurements using BIA technology:

- Nightingale CM, Rudnicka AR, Owen CG, Donin AS, Newton SL, Furness CA, Howard EL, Gillings RD, Wells JC, Cook DG, Whincup PH. **Are ethnic and gender specific equations needed to derive fat free mass from bioelectrical impedance in children of South Asian, Black African-Caribbean and White European origin? Results of the assessment of body composition in children study.** Plos One 2013; 18, 8(10):e76426.
- Kumar S, Khosravi M, Massart A, Potluri M, Davenport A. **The effects of racial differences on body composition and total body water measured by multifrequency bioelectrical impedance analysis influence delivered Kt/V dialysis dosing.** Nephron Clin Pract. 2013;124(1-2):60-6.
- Aglago KE, Menchawy IE, Kari KE, Hamdouchi AE, Barkat A, Bengueddour R, Haloui NE, Mokhtar N, Aguenau H. **Development and validation of bioelectrical impedance analysis equations for predicting total body water and fat-free mass in North-African adults.** Eur J Clin Nutr 2013; 67(10):1081-6.
- Nightingale CM, Rudnicka AR, Owen CG, Cook DG, Whincup PH. **Patterns of body size and adiposity among UK children of South Asian, black African-Caribbean and white European origin: Child Heart And health Study in England (CHASE Study).** Int J Epidemiol 2011; 40(1):33-44.
- Haroun D, Taylor SJ, Viner RM, Hayward RS, Darch TS, Eaton J, Cole TJ, Wells JC. **Validation of Bioelectrical Impedance Analysis in Adolescents Across Different Ethnic Groups.** Obesity 2010; 18(6):1252-59.
- Gibson AL, Holmes JC, Desautels RL, Edmonds LB, Nuudi L. **Ability of new octapolar bioimpedance spectroscopy analyzers to predict 4-component-model percentage body fat in Hispanic, black, and white adults.** Am J Clin Nutr 2008; 87(2):332-8.
- Zhu S, Heymsfield SB, Toyoshima H, Wang Z, Pietrobelli A, Heshka S. **Race ethnicity-specific waist circumference cutoffs for identifying cardiovascular disease risk factors.** Am J Clin Nutr 2005; 81(2): 409-415.
- Deurenberg P, Deurenberg-Yap M, Schouten FJ. **Validity of total and segmental impedance measurements for prediction of body composition across ethnic population groups.** Eur J Clin Nutr 2002; 56:214-220.
- Jakicic JM, Wing RR, Lang W. **Bioelectrical impedance analysis to assess body composition in obese adult women: the effect of ethnicity.** Int J Obes 1998; 22:243-249.
- McKeigue PM, Shah B, Marmot MG. **Relation of central obesity and insulin resistance with high diabetes prevalence and cardiovascular risk in South Asians.** Lancet 1991; 337:382-386.

### To summarize the key findings related to ethnicity and gender:

Previous articles have demonstrated a need for ethnic-and gender-specific prediction equations both in adults and in adolescents. Having in the equation control for ethnicity we reduced the underestimation of fat mass in Asian population.

Ethnic differences in the optimal equations for the prediction of FFM from BIA are likely to reflect the marked ethnic differences in body composition in children of different ethnic groups (Deurenberg P, Deurenberg-Yap, 2002). These include differences in stature, black African-Caribbean children are taller and in particular have greater leg length than white Europeans and South Asians, and lean mass, particularly muscle mass, which tends to be lower among South Asians (Nightingale et al, 2011).

In addition, the amount and distribution of body fat varies appreciably between ethnic groups, with South Asians having a higher proportion of total fat in their abdomen (McKeigue et al 1991), while black African-Caribbeans may have a lower proportion compared to white Europeans (Zhu et al, 2005).





## PHYSICAL ACTIVITY

In addition, Tanita has created Athlete mode to account for differences in muscle mass hydration of standard and more active individuals.

- Verney J, Schwartz C, Amiche S, Pereira B, Thivel D. **Comparisons of a Multi-Frequency Bioelectrical Impedance Analysis to the Dual-Energy X-Ray Absorptiometry Scan in Healthy Young Adults Depending on their Physical Activity Level.** J Hum Kinet. 2015;14(47):73-80.
- Gába A, Kapuš O, Cuberek R, Botek M. **Comparison of multi- and single-frequency bioelectrical impedance analysis with dual-energy X-ray absorptiometry for assessment of body composition in post-menopausal women: effects of body mass index and accelerometer-determined physical activity.** J Hum Nutr Diet. 2015; 28(4):390-400.

### COMMENTS:

Several articles, see references above and also the references in the two articles mentioned (Verney et al, 2015; Gaba et al, 2015) where they underlined the accuracy of BIA depends on level of physical activity. In other words hydration of fat free mass is influenced by physical activity.

In light of this, it is fundamental to know physical activity level and having an equation that “control” for physical activity.




# Levels of Accuracy

## How does BIA technology work?

Bioelectrical Impedance Analysis is a technique used for estimating body composition. All Tanita body composition monitors use advanced Bioelectrical Impedance Analysis technology. When you stand on a Tanita monitor, a very low, safe electrical signal is sent from four metal electrodes through your feet to your legs and abdomen to produce whole body composition measurements. In segmental models, the four hand-held electrodes will provide extra readings for each leg, arm and abdominal area.

The electrical signal passes quickly through water that is present in hydrated muscle tissue but meets resistance when it hits fat tissue. This resistance, known as impedance, is measured and input into scientifically validated Tanita equations to calculate body composition measurements in under 20 seconds.

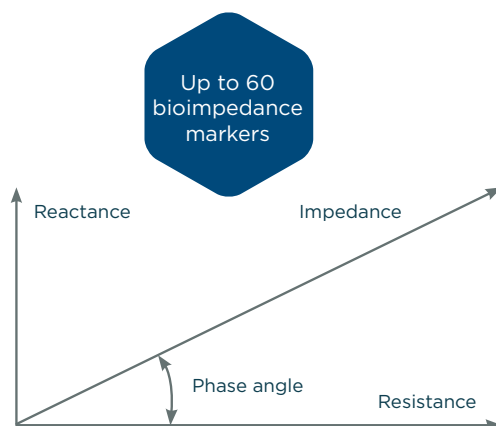


## Multi frequency BIA technology

Tanita Multi-Frequency Monitors are able to measure bioelectrical impedance analysis at three or six different frequencies. The additional frequencies provide an exceptional level of accuracy compared to single and dual frequency monitors. The lower frequencies measure the impedance external to the cell membrane.

The higher frequencies are able to penetrate the cell membrane.

By measuring impedance at both the lower and higher frequencies it is possible to estimate extra-cellular water (ECW), intra-cellular water (ICW) and Total Body Water. This information is essential for providing the health status of a person and indicating health risks such as severe dehydration or oedema.

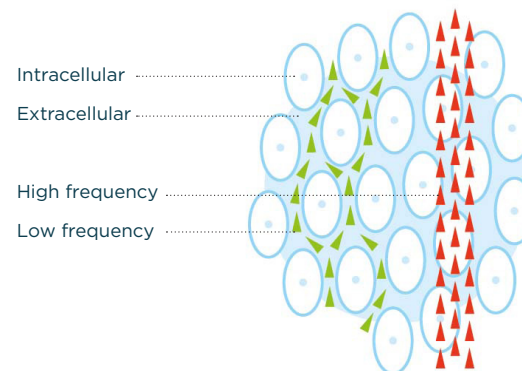


## Single frequency BIA technology

Tanita body composition monitors with Single frequency Bio-electrical Impedance Analysis Technology use a single frequency to capture body composition data.



## Dual frequency BIA technology

Tanita body composition monitors with Advanced Dual Bioelectrical Impedance Analysis Technology use two different frequencies to capture your body composition data. By using different frequencies, a higher accuracy of measurements can be achieved.

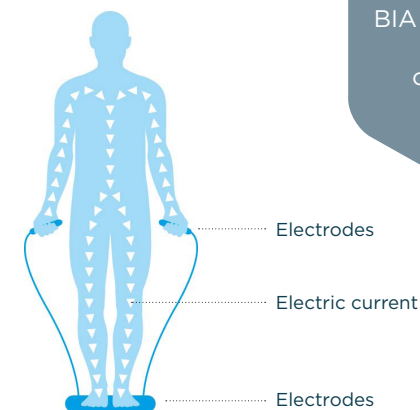

Further detailed information on the benefits of BIA technology in the measurement of body fat can be found at [www.tanita.nl](http://www.tanita.nl)

# Levels of Personalisation



## Segmental Personalisation

**Segmental Body Composition Measurements is the highest level of personalised assessment available.**

In addition to whole body measurements, the Tanita Segmental Monitor will assess impedance of each arm, leg and trunk area independently. This allows an additional layer of information about a person's health and fitness status including segmental muscle mass and fat free mass.

This information can be used to identify specific anomalies in body composition such as oedema in the legs or localized muscle changes pre or post surgery having higher upper body muscle mass. More importantly, segmental body composition analysis allows even the smallest changes in body composition to be identified and monitored over time giving a precise picture of overall health.



## Whole Body Personalisation

**Using Advanced Dual or Single BIA technology, Tanita Body Composition Monitors can provide instant whole body measurements.**

This includes body fat, fat mass, fat free mass, muscle mass, total body water, bone mass, BMR, metabolic age and visceral fat level, plus body cell data such as phase angle. Further analysis of healthy ranges for these parameters are also available providing an excellent overview of a person's health and fitness status.



### BIA Information

|     | 5kHz        | 50kHz       | 250kHz      | Phase Angle |
|-----|-------------|-------------|-------------|-------------|
| H-L | 667.0 -24.3 | 599.3 -57.4 | 539.9 -60.6 | -5.5        |
| RL  | 252.9 -10.4 | 224.6 -22.0 | 203.2 -17.5 | -5.6        |
| LL  | 257.4 -10.5 | 228.7 -22.1 | 206.9 -18.3 | -5.5        |
| RH  | 391.1 -13.7 | 353.4 -35.9 | 314.7 -43.5 | -5.8        |
| LH  | 385.2 -12.6 | 348.8 -33.7 | 313.1 -42.3 | -5.5        |
| L-L | 511.9 -20.8 | 454.7 -44.0 | 410.9 -35.7 | -5.5        |

# Applications of BIA

## Benefits in Nutritional Therapy and Dietetics:

- Accurately assess total body composition and create individualised treatment plans.
- Monitor and preserve lean mass to protect metabolic health, patient mobility and musculoskeletal health.
- Supports the diagnosis and monitoring of Sarcopenia, Cachexia and malnutrition.
- Supports the diagnosis, treatment and monitoring of patients for whom BMI is not appropriate (Bariatrics, Eating Disorders, patients with acute or chronic illness)

## Benefits in Bariatrics:

- Accurately assess total body composition to review the requirement for/effectiveness of intervention.
- Create individualised treatment plans based on patient need.
- Monitor and preserve lean mass after surgery to protect metabolic health, patient mobility and musculoskeletal health.
- Monitor intra/extracellular water to support the detection of post-surgical issues.

## Benefits in Oncology:

- Prehabilitation – Monitor and maintain muscle mass to improve fitness for surgery or treatment, detect and treat Sarcopenia, Cachexia and malnutrition to improve prognosis.
- Treatment – Replace BMI with BIA to reduce toxicity and improve the efficacy of Chemotherapy.
- Rehabilitation – Monitor lean mass and Phase Angle to assess recovery after treatment, improve longer-term prognosis and patient quality of life.

## Benefits in Physiotherapy:

- Detects and monitors the effectiveness of the treatment of muscle imbalance after injury or poor load handling.
- Measures muscle quality, physique rating, leg muscle score and Sarcopenic index to assess the risk of frailty and falls.
- Monitors the effectiveness of rehabilitation plans for patients recovering from accidents, acute illness or neuroglial disease.
- Supports patient motivation and adherence to treatment programmes.

## Benefits in Respiratory Medicine:

- Incorporation of BIA into the diagnosis pathway to better assist the staging of respiratory disease.
- Replace BMI with BIA in the BODE model.
- Detect and treat Sarcopenia and Cachexia to improve patient prognosis.
- Monitor weight gain interventions with a focus on increasing lean mass to protect metabolic and cardiovascular health.



## Benefits in Lifestyle Coaching and Health Improvement:

- Create individual support programmes based on client need.
- Educate clients on holistic health, shifting the focus from weight to reducing fat and maintaining muscle mass.
- Provide reports which help clients understand healthy ranges for measurements to create healthy achievable goals.
- Increase motivation, adherence and goal attainment with a wide range of simple indicators of progress and success.





# USING TANITA TO MEASURE, MONITOR & MOTIVATE

## Professor David Nocca

**Professor of Digestive Surgery  
Head of the bariatric and metabolic surgery unit  
CHU Montpellier (Montpellier University Hospital)**

He is recognized worldwide as an expert in laparoscopic and bariatric surgery and was one of the first to integrate LPG techniques into the pre and postoperative management of the obese patient. He has performed over 2500 bariatric surgeries and, in 2013, developed the cutting edge Nissen-sleeve technique; which has significantly decreased the morbidity of sleeve gastrectomy (less gastro-oesophageal reflux, less fistula).

From his clinic in Montpellier, France; Professor Nocca is also prolific in the field of bariatric training and education, and is the founding President of the French League Against Obesity. Since 2019, he has been an IFSO Ambassador (International Federation for the Surgery of Obesity).



**“ We have been working with Tanita at our Montpellier clinic for around 2 years. The device we have at our clinic is the MC-980 Plus; which is Tanita’s most precise and accurate BIA device.**

Clinical accuracy and precision is particularly important with our patients as they have elements of body composition well outside of healthy norms, and it can be difficult to track these accurately with lower grade devices.

We use bioimpedance analysis to help accurately diagnose and plan the best course of action for our patients, to monitor the efficacy of treatment, and patient adherence to post-surgical support. The analysis provides both BMI and fat mass, which are important indicators of the success of surgical intervention.

The major benefit of incorporating bioimpedance analysis into my practice has been the improvement in metabolic tracking. Bioimpedance analysis considers the patient’s post-surgical lean and muscle mass when calculating BMR; providing a much more accurate estimation of the efficiency of the patient’s metabolism; supporting post-surgical nutritional guidance and long-term weight maintenance.

An unwanted side effect of bariatric surgery can be the loss of lean and muscle mass (Maimoun, L et al, 2017), this can have a detrimental effect upon both the metabolic and musculoskeletal health, and longer-term mobility of the patient. At our Montpellier clinic, we are committed to supporting the long-term holistic health and quality of life of our patients. We have implemented a range of post-surgical interventions to support the maintenance of lean and muscle mass, and we track the efficacy of these using the muscle mass measurement provided by the Tanita analysis.

Another useful measurement, which is unique to the Tanita MC-980, is the Sarcopenia Index which supports the assessment of the patient’s longer-term risk of developing Sarcopenia and allows us to implement preventative strategies.

**Patients’ motivation to continue to work towards improving their health is greatly improved when we can easily share their progress with them, and the Tanita analysis provides useful information and insights which help support the work of my team.** ”



**I AM  
ACHIEVING  
MORE**  
FOR MY CLIENTS





# Information Output

Healthcare professionals are dedicated to achieving long-lasting improvements in health for their clients, and the Tanita pro app can help you achieve more.

Analysing individual and group data on the Tanita pro app will give greater understanding of an individual's health and fitness status, more in-depth analysis of group and individual data and a greater understanding of what results can be achieved.

By accessing clients' body composition data on the Tanita pro app, you have the facts at your fingertips; clear on-screen analysis helps you to show them progress and the impact of their hard work.

Powerful group data analysis allows you to see the results for clients in a specific age group, with specific needs, or for those following a particular programme or diet. This will help to inform the care and input delivered, and ultimately build on success. What's more, you have the data for all your clients in one place, no matter where you are working.

Compatible  
with the  
**MC-780** and  
**MC-580**

Flexible,  
mobile and  
easy to  
use

Cost-effective  
packages  
for up to 200,  
1000 and  
unlimited client  
lists

Download  
and use  
**FREE** for  
up to 10  
clients

Runs  
on **iOS**





# Information Output



## Tanita Pro Software Information Output

The Tanita PRO software package has been developed in partnership with the leading software developer Medizin & Service GmbH.

The software captures data from Tanita Body Composition Analysers, ERKA blood pressure monitor and Activity Monitors, transfers it to a computer, and provides a patient database with professional reports, graphs and trend analysis that can be used for patient education, research and clinical records.

In line with EU regulations, the software is Medically Approved, which complies with MDD (Medical Device Directive) regulations. (Council Directive 93/42/EEC of 14 June 1993 concerning medical devices.)

In addition to body composition data captured from the Tanita Analyser, the user can input target values and waist circumference measurements allowing a full overview of a patient's health and physical progress.

A full colour, printable, client consultation sheet showing segmental body composition analysis and ranges is available for our full Tanita Professional Range.

Please note: suitable for Windows



# TANITA PRO

| CUSTOMER ID | NAME       | FIRST NAME | DATE OF BIRTH | SEX | CITY |
|-------------|------------|------------|---------------|-----|------|
| demo02      | Beispiel   | Erna       | 17.07.1967    | F   |      |
| k0021       | Blasi      | Vinicio    | 14.03.1953    | M   |      |
| k0011       | Brandauer  |            | 13.03.1958    | F   |      |
| k0005       | Horrer     | Stefan     | 20.09.1972    | M   |      |
| waetz_k0015 | Japirak    | Madriga    | 04.04.1936    | F   |      |
| demo01      | Muffler    | Ernst      | 16.05.1964    | M   |      |
| k0023       | Simonc     | Manfred    | 08.11.1967    | M   |      |
| k0022       | Stadtbauer | Alfred     | 05.03.1956    | M   |      |
| demo03      | Test       | Anne       | 07.03.1975    | F   |      |
| demo04      | Versuch    | Amie       | 11.08.1988    | M   |      |
| k0013       | Albert     |            | 09.09.1980    | M   |      |
| k0014       | Alex       |            | 19.08.1988    | M   |      |
| k0017       | Andreas    |            | 25.05.1984    | M   |      |
| k0019       | Anna       |            | 08.10.1987    | F   |      |
| k0009       | Brigit     |            | 03.10.1989    | F   |      |
| k0010       | Christine  |            | 23.11.1990    | F   |      |
| k0020       | Christoph  |            | 26.01.1984    | M   |      |



# Body Composition Measurements



## Weight



## Body Fat Mass

The actual weight of fat in your body



## Body Fat Percentage

The amount of body fat as a proportion of your body weight



## Total Body Water Percentage

The total amount of fluid in your body as percentage of your total weight



## Muscle Mass

The predicted weight of muscle in your body including skeletal muscles, smooth muscles and the water contained within your muscles



## Physique Rating

Assesses your physique according to the ratio of body fat and muscle mass in the body



## Daily Caloric Intake

Estimate of calories you can eat in 24 hours to maintain current weight



## BMR (Basal Metabolic Rate)

Number of calories your body needs at rest



## Metabolic Age

Age level your body is rated at, according to your BMR



## Bone Mass

The amount of bone (bone mineral level, calcium, other minerals) in your body



## Visceral Fat Rating

Indicates level of fat surrounding your vital organs in the abdominal area



## Muscle Score

Muscle mass is judged by calculating the amount of muscle mass against your height and then the amount is classified.



## Body Mass Index

Indicates the relationship between your height and weight



## Phase Angle

Phase angle is an indicator of cellular health and integrity.



## ICW

Intracellular Water is the fluid found inside cells. Usually 40% of your body weight is intracellular water



## ECW

Extracellular Water is the body fluid found outside of cells.



## Protein

The weight of protein in the body, protein is essential for the maintenance of muscle within the body



## Segmental Analyses of body fat and muscle mass

Body fat and muscle are analysed segmentally in order to assess fat and muscle distribution



## Sarcopenic Index

A risk indicator for the individual developing Sarcopenia





## %Total Body Water

**Female** 45% to 60%  
**Male** 50% to 65%  
**Athletic Body Types**  
 5% higher than adult range



## Visceral Fat

**Healthy level rating** (1 - 12)  
**Excess level rating** (13 - 59)



## Healthy Body Fat Range %

|                   | Underfat | Healthy   | Overfat   | Obese |
|-------------------|----------|-----------|-----------|-------|
| <b>Female Age</b> |          |           |           |       |
| 20 - 39           | 0% - 21% | 21% - 33% | 33% - 39% | 39%+  |
| 40 - 59           | 0% - 23% | 23% - 34% | 34% - 40% | 40%+  |
| 60 - 99           | 0% - 24% | 24% - 36% | 36% - 42% | 42%+  |
| <b>Male Age</b>   |          |           |           |       |
| 20 - 39           | 0% - 8%  | 8% - 19%  | 19% - 25% | 25%+  |
| 40 - 59           | 0% - 11% | 11% - 21% | 21% - 28% | 28%+  |
| 60 - 99           | 0% - 13% | 13% - 25% | 25% - 30% | 30%+  |



## BMI

**Healthy range**  
 18.5 - 25




## Muscle Mass Score

Muscle mass is judged calculating the amount of muscle mass against the person's height and then the amount is classified.



## Phase Angle

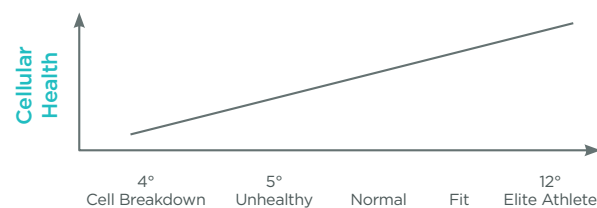


### Preferred Phase Angle

5° Female  
 6° Male  
 10° Adolescent  
 12° Athletic



## Physique Rating


| Result | Physique Range            | Explanation                                |
|--------|---------------------------|--|
| 1      | Hidden Overfat            | High body fat % with low muscle mass       |
| 2      | Medium Frame Overfat      | High body fat %, moderate muscle mass      |
| 3      | Solidly Built             | Large frame, high body fat % & muscle mass |
| 4      | Low Muscle                | Average body fat % & low muscle mass       |
| 5      | Standard                  | Average levels of body fat % & muscle mass |
| 6      | Muscular                  | Average body fat % & high muscle mass      |
| 7      | Low Muscle & Underfat     | Low body fat % & low muscle mass           |
| 8      | Thin & Muscular (Athlete) | Low body fat % & adequate muscle mass      |
| 9      | Very Muscular (Athlete)   | Low body fat % & high muscle mass          |

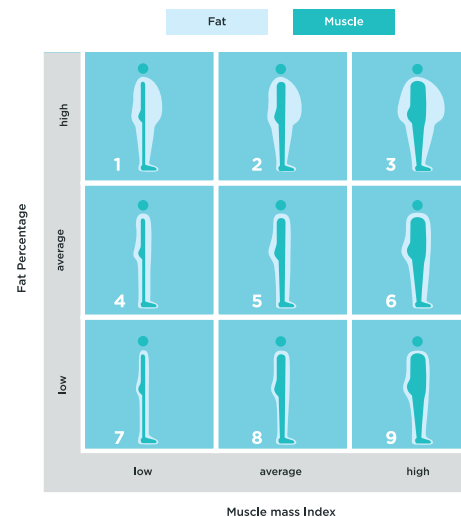


## Segmental Measurements

8-electrode segmental technology to show body composition measurements for each arm, leg and trunk area.

### Segmental fat analysis

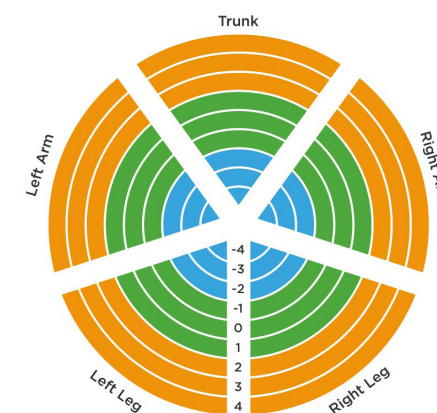

### Segmental muscle analysis

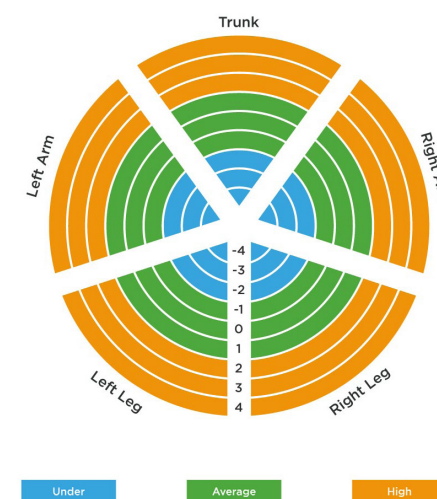



## MC-980 MA PLUS

Segmental Multi Frequency  
Body Composition Analyser  
with touchscreen display and  
Windows® OS

The MC-980 MA PLUS is the ultimate tool in providing fast in-depth information for truly personalised medical, health and weight management consultations. Incorporating the latest multi-frequency BIA technology with the flexibility of in-built Microsoft® Windows® real time OS software, this monitor provides fast, convenient and accurate information. The MC-980 MA PLUS provides a full medical grade body composition analysis in less than 30 seconds and has an easy-to-follow colour interactive touch screen display.



MC-980 MA PLUS



## LEVEL OF COMPLIANCE


- Accuracy grade: NAWI Class III
- Medical Device Classification: MDD Class II-a

## LEVEL OF PERSONALISATION

- Full segmental body composition analysis provided in 30 seconds using clinically accurate Tanita Multi Frequency BIA Technology.
- The Tanita device can be operated effortlessly using the intuitive touchscreen display which presents precise Tanita BIA data and allows easy transfer of results to PC or printer.

## INFORMATION OUTPUT

- Software and detailed consultation sheets available in 14 languages.
- In-built Microsoft® Windows® real time OS allows client data to be automatically stored, managed and output. Windows 8 upgrade.
- USB ports allow simple data input/output and accessories to be connected including printers, bar code scanners and data capture devices.
- Tanita PRO Software compatible, allowing trend analysis, health risk assessments and full data management.

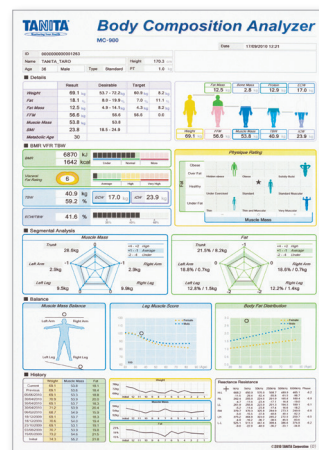

MC-980 MA PLUS  
print out



## Total Body Measurements

- Weight
- BMI
- Body Fat %
- Visceral Fat Indicator
- Fat Mass
- Fat Free Mass
- Muscle Mass
- Protein kg
- Total Body Water Kg
- Total Body Water %
- Extra-Cellular Water Kg
- Intra-Cellular Water Kg
- ECW/TBW Ratio
- Basal Metabolic Rate
- Basal Metabolic Rate Indicator
- Bone Mineral Mass Indicator
- Metabolic Age
- Physique Rating
- Phase angle
- Sarcopenia Index \*new\*

## Segmental Measurements

- Segmental Body Fat %
- Segmental Body Fat kg
- Segmental Fat Distribution Analysis
- Segment Fat Distribution Rating
- Segmental Muscle Mass Kg
- Segmental Muscle Mass Rating
- Segmental Muscle Mass Balance
- Leg Muscle Score
- Segmental Reactance/Resistance
- Segmental Phase Angle

## Information output

TANITA  
PRO



5 YEAR  
GUARANTEE



TANITA



## Clinical Application

|                 |   |                   |   |                     |   |                            |   |               |   |
|-----------------|---|-------------------|---|---------------------|---|----------------------------|---|---------------|---|
| Oncology        | ✓ | Weight Management | ✓ | Occupational Health | ✓ | Pharmacy                   | ✓ | Physiotherapy | ✓ |
| Diabetes        | ✓ | Renal             | ✓ | Bariatrics          | ✓ | Paediatrics                | ✓ |               |   |
| Cystic Fibrosis | ✓ | COPD              | ✓ | General practice    | ✓ | Geriatrics / Active ageing | ✓ |               |   |

## Technical Specification

|                               |                       |
|-------------------------------|-----------------------|
| Accuracy Grade                | NAWI Class III        |
| Medical Device Classification | <b>MDD Class II-a</b> |
| Age Range                     | 5 - 99 years          |
| Weight Capacity               | 300 kg                |
| Graduation                    | 0.1kg                 |
| Product Dimensions            | 450 x 490 x 1240 mm   |
| Product Weight                | 33 kg                 |
| Power Source                  | 230V                  |
| Interface                     | 3 x USB               |





## MC-780 MA

Multi frequency Segmental Body Composition Analyser with interactive display console and in-built SD card facility

The MC-780 MA has been designed to be an interactive stand-alone unit where clients can step on and take a measurement without specialist assistance. A full segmental body composition analysis is performed in less than 20 seconds.

The large LED dual display shows whole body composition measurement data and detailed segmental analysis in an easy-to-read illustrative format.



MC-780 MA S



MC-780 MA P



TANITA  
**PRO**  
APP



## LEVEL OF COMPLIANCE

- Accuracy grade: NAWI Class III
- Medical Device Classification: MDD Class II-a

## LEVEL OF PERSONALISATION

- Full and fast segmental body composition analysis using clinically accurate multi frequency BIA technology.
- Certified for medical consultations.

## INFORMATION OUTPUT


- In-built SD card facility allows data to be automatically collected and downloaded at convenience
- Client Identity feature allows continuous data to be collected for each client effortlessly. Also allows large anonymous data sets to be collated for research studies
- USB Connection
- Display console can be reversed for confidential readings with children or when large obese clients step on
- Output to any Pictbridge printer for a detailed client consultation sheet allowing a full client assessment.

## Clinical Application

|                 |   |                   |   |                     |   |                            |   |               |   |
|-----------------|---|-------------------|---|---------------------|---|----------------------------|---|---------------|---|
| Oncology        | ✓ | Weight Management | ✓ | Occupational Health | ✓ | Pharmacy                   | ✓ | Physiotherapy | ✓ |
| Diabetes        | ✓ | Renal             | ✓ | Bariatrics          | ✓ | Paediatrics                | ✓ |               |   |
| Cystic Fibrosis | ✓ | COPD              | ✓ | General practice    | ✓ | Geriatrics / Active ageing | ✓ |               |   |

## Technical Specification

|                               |   |
|-------------------------------|---|
| Accuracy Grade                | NAWI Class III                                |
| Medical Device Classification | <b>MDD Class II-a</b>                         |
| Age Range                     | 5 - 99 years                                  |
| Weight Capacity               | 270kg   |
| Graduation                    | 0.1kg   |
| Product Dimensions            | (P) 360 x 360 x 1165mm (S) 360 x 360 x 1165mm |
| Product Weight                | (P) 22kg (S) 15.5kg                           |
| Power Source                  | AC 100 - 240V                                 |
| Interface                     | RS232, USB, SD CARD                           |

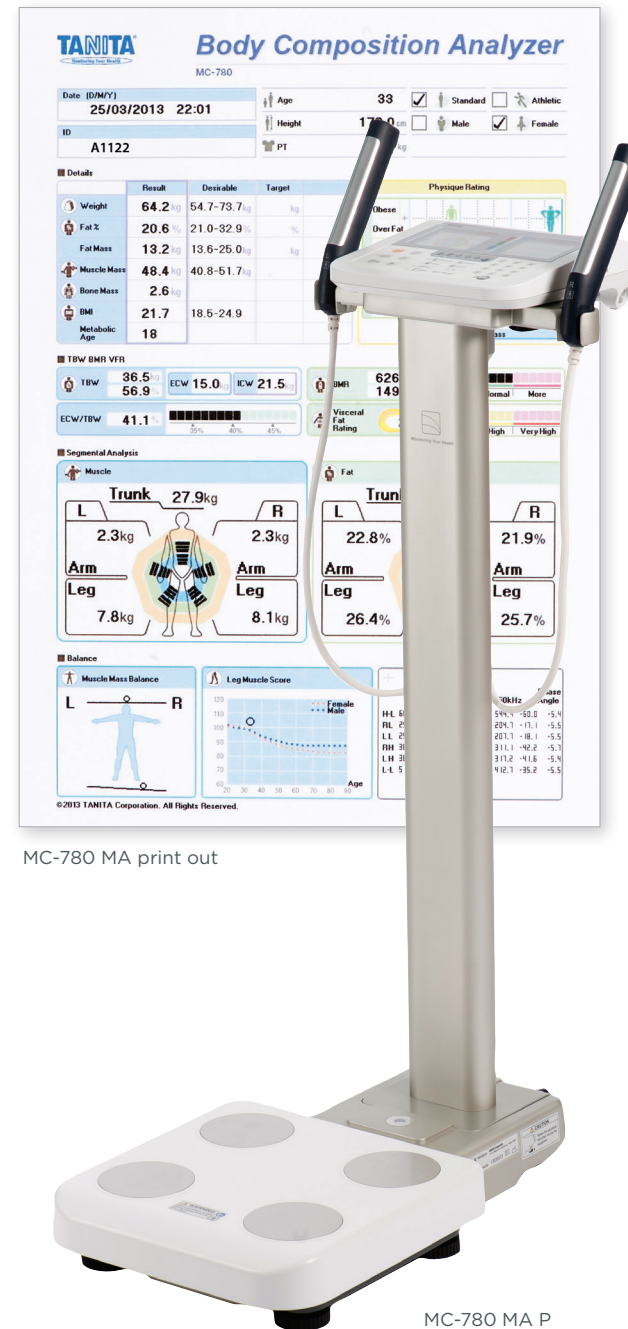

MC-780 MA print out

MC-780 MA P

## Total Body Measurements

- Weight
- BMI
- Body Fat %
- Visceral Fat Indicator
- Fat Mass
- Fat Free Mass
- Muscle Mass
- Physique Rating
- Total Body Water Kg
- Total Body Water %
- Extra-Cellular Water Kg
- Intra-Cellular Water Kg
- ECW/TBW Ratio
- Phase Angle
- Basal Metabolic Rate
- Basal Metabolic Rate Indicator
- Metabolic Age
- Bone Mineral Mass Indicator

## Segmental Measurements

- Segmental Body Fat %
- Segmental Fat Distribution Rating
- Segmental Muscle Mass Kg
- Segmental Muscle Mass Rating
- Segmental Muscle Mass Balance
- Segmental Reactance/Resistance
- Segmental Leg Muscle Score
- Segmental Phase Angle

## Extra measurements only available via software

- Sarcopenic index

## Information output

TANITA  
**PRO**



MADE IN  
**JAPAN**

**5 YEAR  
GUARANTEE**







## MC-580

### Segmental Multi-Frequency Body Composition Analyser with Integrated Bluetooth

This portable body composition monitor MC-580 is the perfect device for client consultations on the move. As it is battery powered, it gives you the ability to use it wherever you want.

It provides instant analysis of a client's health and fitness status as well as monitoring their progress over time, which enables you to provide your client with personalised advice about their training and diet.

The LCD screen shows data for fat and muscle mass & %, including segmental analysis, plus your weight and BMI. All body composition data can then be sent wirelessly to a tablet using integrated Bluetooth. It is compatible with both the Tanita PRO app as well as the Tanita Pro Windows software, which allows you to save, analyse and share body composition results with all clients.



MC-580 S

MC-580 P



## LEVEL OF COMPLIANCE

- Latest dual frequency 4C reactance technology
- Reactance/Resistance technology. Accuracy proven by validation paper from Pennington Biomedical Research Center (Louisiana State University)

## LEVEL OF PERSONALISATION

- Full and fast segmental body composition measurements using the latest multi frequency BIA technology

## INFORMATION OUTPUT

- Segmental data available on the thermal printer
- Segmental fat mass & total fat mass+ segmental muscle mass and total muscle mass directly shown on display
- Extra large LCD dual display shows analysis in an easy-to-read format
- Automatic data transfer through wireless Bluetooth connection to pad and Android tablet.
- Connection to thermal printer via cable

## OTHER FEATURES

- In combination with App or Software, Phase angle is shown which gives an instant assessment of the nutritional state and muscle quality
- Lightweight and portable, suitable for mobile assessments

## Technical Specification

|                    |  |
|--------------------|--|
| Age Range          | 5 - 99 years                                   |
| Weight Capacity    | 270 kg   |
| Graduation         | 100g   |
| Product Dimensions | (P) 395 x 390 x 1027mm<br>(S) 395 x 390 x 67mm |
| Product Weight     | (P) 11.2kg (S) 8.3kg                           |
| Power Source       | 9 V Adapter or 4 x AA Batteries                |
| Interface          | RS-232C  |



\* not included

## Total Body Measurements

- Weight
- Body Fat Mass
- Total Body Water %
- Muscle Mass
- Physique Rating
- Bone Mineral Mass
- Basal Metabolic Rate
- Metabolic Age
- Body Mass Index
- Visceral Fat
- Phase Angle (in combination with App or Software)

## Segmental Measurements

- Segmental Body Fat %
- Segmental Fat Distribution Rating
- Segmental Muscle Mass Kg
- Segmental Muscle Mass Rating
- Segmental Muscle Mass Balance
- Segmental Reactance/Resistance
- Segmental Leg Muscle Score
- Segmental Phase Angle

## Extra measurements only available via software

- Sarcopenic index
- Phase angle
- BMI
- Fat Free Mass
- Body Water Mass

## Information output

TANITA  
**PRO**



**3 YEAR  
GUARANTEE**



# DC-430 MA

## Dual Frequency Body Composition Monitor with Integrated Printer

Featuring Dual Frequency BIA technology, the DC-430 MA delivers full body composition analysis in 15 seconds. Results are instantly shown on the easy-to-read LCD screen and the integrated printer automatically prints the body composition measurements together with a top line analysis.

For large data collection and convenience, all data can be stored on the SD Card for future use. Combined with Tanita PRO Software, the DC-430 MA allows you to conduct client trend analysis, health risk assessments and full data management. In addition, the DC-430 MA has been accredited with the accuracy grade MDD Class II-a and NAWI Class III allowing use for medical consultations.



DC-430 MA S

DC-430 MA P



## LEVEL OF COMPLIANCE

- Accuracy grade: NAWI Class III
- Medical Device Classification: MDD Class II-a

## LEVEL OF PERSONALISATION

- Full body composition analysis provided in 20 seconds using clinically accurate Tanita Dual Frequency BIA Technology
- Certified for medical consultations

## INFORMATION OUTPUT

- Integrated printer prints instant read out of results with topline analysis.
- Results automatically stored on the SD Card, sent to a PC or printed.
- Tanita PRO Software compatible, allowing trend analysis, health risk assessments and full data management.
- Print Out Analysis: Body Fat Analysis, Muscle Mass Indicator, BMR Indicator, Physique Rating, Target: BF and Weight

## CLINICAL APPLICATION

|                 |                     |                       |                              |               |
|-----------------|---------------------|-----------------------|------------------------------|---------------|
| Oncology ✓      | Weight Management ✓ | Occupational Health ✓ | Pharmacy ✓                   | Physiotherapy |
| Diabetes        | Renal               | Bariatrics ✓          | Paediatrics ✓                |               |
| Cistic Fibrosis | COPD                | General practice ✓    | Geriatrics / Active ageing ✓ |               |

## TECHNICAL SPECIFICATION

|                               |  |
|-------------------------------|--|
| Accuracy Grade                | NAWI Class III                             |
| Medical Device Classification | <b>MDD Class II-a</b>                      |
| Age Range                     | 5 - 99 years                               |
| Weight Capacity               | 270kg                                      |
| Graduation                    | 100g                                       |
| Product Dimensions            | (P) 360 x 360 x 1070<br>(S) 360 x 360 x 94 |
| Product Weight                | (P) 13.5kg<br>(S) 7kg                      |
| Power Source                  | AC 100 - 240V                              |
| Interface                     | RS232, USB, SD CARD                        |



## Measurements

- Body fat %
- Fat mass kg,
- Fat free mass kg
- Muscle mass kg
- Total Body Water %
- Body mass index
- Bone mass kg
- Physique rating
- Visceral fat rating
- Basal Metabolic Rate kcal
- Basal Metabolic Rate indicator
- Metabolic Age
- Print Out Analysis:
  - Body Fat Analysis
  - Muscle Mass Indicator
  - BMR Indicator
  - Physique Rating
  - Target: BF and Weight

## Extra measurements only available via software

- Phase angle

## Accessories



TP-301  
Paper Rolls



Bluetooth wireless  
connection Parani

## Information output

**TANITA**  
**PRO**

MADE IN  
**JAPAN**

**3 YEAR**  
**GUARANTEE**

**M**  
**III**





## DC-360

### Dual Frequency Body Composition Monitor with Integrated Printer

Featuring Dual Frequency BIA technology, the DC-360 delivers full body composition analysis in 20 seconds. Results are instantly shown on the easy-to-read LCD screen and the integrated printer automatically prints the body composition measurements together with a top line analysis.

The robust, low profile platform provides additional client stability. For large data collection and convenience, all data can be stored on the SD Card for future use. Compatible with Tanita PRO Software, the DC-360 allows client trend analysis, health risk assessments and full data management.



DC-360

## LEVEL OF PERSONALISATION

- Full body composition analysis provided in 20 seconds using clinically accurate Tanita Dual Frequency BIA Technology

## INFORMATION OUTPUT

- Integrated printer provides instant read out of results with topline analysis.
- Results automatically stored on the SD Card, sent to a PC or printed.
- Tanita PRO Software compatible, allowing trend analysis, health risk assessments and full data management.

## CLINICAL APPLICATION

|                 |                     |                       |                            |               |
|-----------------|---------------------|-----------------------|----------------------------|---------------|
| Oncology        | Weight Management ✓ | Occupational Health ✓ | Pharmacy                   | Physiotherapy |
| Diabetes        | Renal               | Bariatrics            | Paediatrics                |               |
| Cystic Fibrosis | COPD                | General practice      | Geriatrics / Active ageing |               |

## TECHNICAL SPECIFICATION

|                    |  |
|--------------------|--|
| Age Range          | 5 - 99 years                               |
| Weight Capacity    | 270kg                                      |
| Graduation         | 100g                                       |
| Product Dimensions | (P) 360 x 360 x 1070<br>(S) 360 x 360 x 94 |
| Product Weight     | (P) 13.5kg<br>(S) 7kg                      |
| Power Source       | AC 100 - 240V                              |
| Interface          | RS232, USB, SD CARD                        |

**TANITA**  
BODY COMPOSITION ANALYZER  
DC-360

26/JAN/2020 20:59

INPUT  
ID No. 000001234567890  
BODY TYPE STANDARD  
GENDER MALE  
AGE 35  
HEIGHT 180 cm  
CLOTHES WEIGHT 1.5kg

RESULT  
WEIGHT 89.0kg  
FAT % 25.9 %  
FAT MASS 21.5kg  
FFM 61.5kg  
MUSCLE MASS 58.4kg  
TBW 48.4kg  
TBW % 54.3 %  
BONE MASS 3.1kg  
BMR 7598 kJ  
1816kcal  
METABOLIC AGE 50  
VISCERAL FAT RATING 8

BMI 25.6  
IDEAL BODY WEIGHT 71.3kg  
DEGREE OF OBESITY 16.4 %

DESIRED RANGE  
FAT % 8.0 - 19.9 %  
FAT MASS 5.3 - 15.3kg

TARGET  
TARGET BFX is: 15 %  
Predicted weight: 72.4kg  
Predicted fat mass: 10.9kg  
FAT TO LOSE: 10.6kg

Consult your physician before beginning any weight management program. Tanita is not responsible for determining your target BFX.

INDICATOR  
\*FAT %  
- | 0 | + | ++  
\*BMI  
- | 0 | + | ++  
\*VISCERAL FAT RATING  
113  
\*MUSCLE MASS  
- | 0 | +  
\*BMR  
- | 0 | +  
\*PHYSIQUE RATING  
OBESE

\*BIOELECTRICAL DATA  
6.25kHz 50kHz  
R 439.5 394.3  
X -18.3 -28.0



DC-360 S



## Measurements

- Body fat %
- Fat mass kg,
- Fat free mass kg
- Muscle mass kg
- Total Body Water %
- Body mass index
- Bone mass kg
- Physique rating
- Visceral fat rating
- Basal Metabolic Rate kcal
- Basal Metabolic Rate indicator
- Metabolic Age
- Print Out Analysis:
  - Body Fat Analysis
  - Muscle Mass Indicator
  - BMR Indicator
  - Physique Rating
  - Target: BF and Weight

## Extra measurements only available via software

- Phase angle

## Accessories



TP-301  
Paper Rolls



Bluetooth wireless  
connection Parani

## Information output

**TANITA**  
**PRO**

MADE IN  
JAPAN

**3 YEAR**  
**GUARANTEE**





# DC-240 MA

Portable, high capacity medical grade body composition monitor with dual frequency reactance BIA technology

The DC-240 MA offers the latest Dual Frequency Reactance BIA technology in the lightest medically approved body composition monitor, weighing just 4.7kg.

It has been developed with input from healthcare, fitness and weight management professionals and its portability makes it ideal for mobile consultations, community work or field research studies.

It displays weight, body fat %, body water % and BMI readings on the oversized, easy to read display.

When combined with our Tanita Pro software, it provides 8 additional measurements, such as muscle mass, visceral fat and basal metabolic rate.

The Tanita Pro software, allows for automatic set-up for personalised patient studies, capturing measurements and trend results in a variety of reporting formats.



DC-240 MA



## LEVEL OF COMPLIANCE

- Accuracy grade: NAWI Class III
- Medical Device Classification: MDD Class II-a

## LEVEL OF PERSONALISATION

- The Tanita Pro software, allows for automatic set-up for personalised patient studies, capturing measurements and trend results in a variety of reporting formats.

## INFORMATION OUTPUT

- Core body composition results shown on screen. All additional results can be accessed via Tanita PRO Software allowing trend analysis, health risk assessments and full data management.

## OTHER FEATURES

- Lightweight and highly portable (4.7kg) perfect for field studies, mobile and community assessments
- Low profile platform for additional stability
- Dual-frequency 4 electrode
- High weight capacity 200kg
- Calibrated up to 300,000 uses with automatic calibration after each measurement

## TECHNICAL SPECIFICATION

|                               |   |
|-------------------------------|---|
| Accuracy Grade                | NAWI Class III                              |
| Medical Device Classification | <b>MDD Class II-a</b>                       |
| Age Range                     | 5 - 99 years                                |
| Weight Capacity               | 200kg                                       |
| Graduation                    | 100g  |
| Product Dimensions            | 340 x 440 x 65 mm                           |
| Product Weight                | 4.7kg                                       |
| Power Source                  | Battery: 9 V Adaptor<br>or 6 x AA Batteries |
| Interface                     | USB   |



DC-240 MA

## Measurements

- Weight
- Body fat %
- Body water %
- BMI

## Extra measurements only available via software

- Body Fat %
- BMI
- Fat Mass
- Fat Free Mass
- Body Water %
- Body Water Mass
- Muscle Mass
- Bone Mineral Mass
- Visceral Fat Level
- Basal Metabolic Rate
- Metabolic Age
- Phase angle

## Accessories



C-300 CH Bag

## Information output

**TANITA**  
**PRO**

MADE IN  
**JAPAN**

**3 YEAR**  
**GUARANTEE**







# WB-150 MA

## High Capacity Scale

The WB-150MA scale incorporates single load cell precision weighing up to 270kg.

The extra large digital display is easy to read. Additional functions include a tare function useful for weighing small children held in an adult's arms.

The scale is available in a column version or a portable version.



WB-150 MA S

WB-150 MA P



### LEVEL OF COMPLIANCE

- Accuracy grade: NAWI Class III
- Medical Device Classification: MDD Class II-a

### INFORMATION OUTPUT

- Easy to read extra large digital display

### OTHER FEATURES

- High weight capacity 270kg
- Tare and weight lock facility
- Calibrated up to 300,000 uses with automatic calibration after each measurement

### TECHNICAL SPECIFICATION

|                               |  |
|-------------------------------|--|
| Accuracy Grade                | NAWI Class III   |
| Medical Device Classification | <b>MDD Class II-a</b>                                  |
| Weight Capacity               | 270 kg   |
| Graduation                    | 100 g  |
| Product Dimensions            | (P) 301x 336x 845 mm<br>(S) 301 x 336 x 82 mm          |
| Product Weight                | (P) 7.1kg<br>(S) 5.1 kg                                |
| Power Source                  | DC 9V Adaptor Included or<br>6 x AA Alkaline Batteries |
| Battery life                  | 100 hours continuous use                               |
| Output data                   | RS232C   |
| Warranty                      | 3 Years  |



WB-150 MA P

### Measurements

- Weight
- Tare Facility
- Weight Lock

### Information output

**TANITA**  
**PRO**



**3 YEAR**  
**GUARANTEE**





# WB-380

## Digital Weighing Scale

The WB-380 is a 300kg high capacity precision digital scale featuring a BMI function.

The scale is available in three formats: portable, with a column mounted display or with an integrated height rod.



Column  
Mounted

With  
Remote  
Display

WB-380 S

WB-380 P



## INFORMATION OUTPUT

- Large easy-to-read LCD display
- Rotating display allowing confidential readings

## OTHER FEATURES

- High weight capacity 300kg
- Step on activation
- Low level, stable platform for elderly or obese patients

## TECHNICAL SPECIFICATION

|                       |   |
|-----------------------|---|
| Maximum Capacity      | 300kg   |
| Minimum Graduation    | 0.1kg   |
| Measurement System    | Mechanical Height Rod (WB-380 H only)   |
| Range of Height       | 64cm - 214cm (WB-380 H only)  |
| Input items - Height  | 61cm- 250cm 1cm increments  |
| Output Items - Weight | 300kg / 0.1kg increments  |
| Output Items - Height | 61cm- 250cm / 1cm increments  |
| Output Items - BMI    | 0.1 increments  |
| Overall size          | S: 240 x 139 x 123 mm (Indicator)<br>P: 395 x 595 x 1196 mm<br>H: 395 x 552 x 1425 mm |
| Platform size:        | 395 x 390 x 59 mm   |
| Product Weight        | S: Total 7.1kg<br>P: Total 10.0kg<br>H: Total 11.2kg                                  |
| Output Data Interface | RS-232C (D sub 9-pin Female connector) USB (B-type)                                   |
| Power Source          | AC adapter (included) Centre Minus<br>DC 6V 200mA (LR6 - AA Alkaline Battery x 4)     |
| Battery Life          | Approximately 100 hours of continuous use   |
| Warranty              | 3 years   |



## Measurements

- Weight
- Weight Lock
- BMI
- Height

## Accessories



C-300 Bag

## Information output

**TANITA**  
**PRO**

**3 YEAR**  
**GUARANTEE**

# Accessories



## C-360

Padded Case with Wheels and Telescopic handle

- Compatible with DC-360 S
- Trolley Bag with wheels and pull up handle.
- Dimensions (inc wheels): H:69 x L:43.5 x W:20 cm



## C-430

Padded Case with Wheels and Telescopic handle

- Compatible with Tanita DC-430
- Dimensions (inc wheels): H:54 x L:39 x W: 19.5 cm



## C-780

Padded Case with Wheels and Telescopic handle

- Compatible with MC-780 MA S
- Padded Case with Wheels and Telescopic handle
- Padded interior for safe storage and handy internal pockets.
- Dimensions (incl wheels): H:69 x L:43.5 x W:27 cm



## C-300 CH

Padded Case with Wheels and Telescopic handle

- Compatible with DC-240 and WB-380.
- Total Handle Length - 830 mm.
- Dimensions (inc wheels): 470 x 410 x 245 mm.



## Bluetooth Adapter

- Bluetooth adapter to wirelessly connect Tanita Professional devices



# Payment options

## Leasing

Tanita now offers favourable leasing contracts for professional equipment. We offer leasing contracts ranging from 24 to 72 months with a possible “buying” option.

All we need to be able to help you to expand your business is:

- Company name and country
- Your name, email and title
- Chamber of Commerce number
- Your (business) phone number

Please choose your plan

We'll get in contact with a detailed personal offer within 48 hours

MC-980MA PLUS | €15.500,00

Select duration of lease

3 years | 570.15 p/m

Email address

Organization

Telephone number

Chamber of Commerce no.

Full name

SEND REQUEST



5 YEAR GUARANTEE

**Rick Kaale**

Sales Executive Benelux

[rick.kaale@tanita.eu](mailto:rick.kaale@tanita.eu)

+31 (0)6 18 41 88 74



For more  
information  
contact our  
sales rep

## TANITA PAYMENT PLAN

## 50% IN ADVANCE »» THE REST IN 3 STEPS

We now offer you a new step-by-step payment plan\* that allows you to incorporate body composition analysis into your practice in a budget friendly manner.

### How can you benefit from this:

- **Improve your patients/clients understanding of their body health**, instead of just weight and BMI by measuring full body composition.
- **Motivate your patient/client** with our reports, including ideal values and objectives, which offer a clear overview of the results and changes over time.
- **Celebrate more small successes** with your patients/clients on their journey.

\*The Tanita payment plan has zero interest and no additional charges.

\*\*A direct debit mandate is required when ordering the device. Payment plan applies to a selected range of products.



### HOW IT WORKS:

**1. Select the Tanita BIA monitor that best suits your practice and only pay 50% in advance**

**2. Easily set up your chosen BIA monitor with the expert guidance and training of our dedicated team**

**3. Simply pay the three remaining monthly payments via direct debit\*\***

## Notes



A photograph of an elderly couple standing outdoors in a park-like setting. The woman in the foreground has short, styled white hair and is wearing a teal-colored short-sleeved top. She is smiling warmly at the camera. Behind her, slightly out of focus, is an elderly man with white hair wearing a dark blue t-shirt, also smiling. The background consists of lush green trees and foliage, with sunlight filtering through to create a bokeh effect of soft, glowing circles.

# HEALTHY HABITS FOR HAPPINESS



**Would you like a free demonstration,  
to discuss the clinical application  
or to get a non obligation offer?  
Contact our Tanita team.**

**Europe Office**

Tanita Europe BV  
Hoogoorddreef 56E  
1101 BE AMSTERDAM  
The Netherlands

+31 (0)20 560 29 70  
info@tanita.eu

**[www.tanita.nl](http://www.tanita.nl)**