


# Operating manual

## Recirculating Coolers

FL7006      FLW7006

FL11006    FLW11006

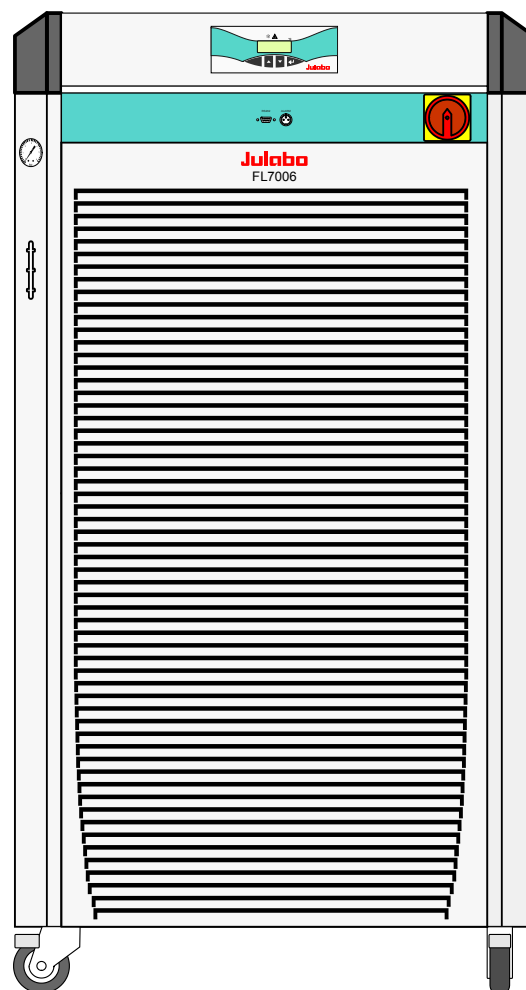

**Julabo**  
THE TEMPERATURE CONTROL COMPANY

JULABO GmbH  
77960 Seelbach / Germany  
Tel. +49 (0) 7823 / 51-0  
Fax +49 (0) 7823 / 24 91  
[info.de@julabo.com](mailto:info.de@julabo.com)  
[www.julabo.com](http://www.julabo.com)

1.951.4828-V5

09/16

1.800.561.8187

[www.itm.com](http://www.itm.com)

[information@itm.com](mailto:information@itm.com)

## Congratulations!

You have made an excellent choice.

JULABO thanks you for the trust you have placed in us.

This operating manual has been designed to help you gain an understanding of the operation and possible applications of our circulators. For optimal utilization of all functions, we recommend that you thoroughly study this manual prior to beginning operation.

## The JULABO Quality Management System



Temperature control devices for research and industry are developed, produced, and distributed according to the requirements of ISO 9001 and ISO 14001. Certificate Registration No. 01 100044846

## Unpacking and inspecting



Unpack the recirculating cooler and accessories and check for damages incurred during transit. These should be reported to the responsible carrier, railway, or postal authority, and a request for a damage report should be made. These instructions must be followed fully for us to guarantee our full support of your claim for protecting against loss from concealed damage. The form required for filing such a claim will be provided by the carrier.

← Lifting device for transportation by crane see page **Fehler! Textmarke nicht definiert.**

Printed in Germany

Changes without prior notification reserved

**Important:** keep original operating manual for future use

## TABLE OF CONTENTS

|                                                                    |                                           |
|--------------------------------------------------------------------|-------------------------------------------|
| 1. Intended use.....                                               | 4                                         |
| 1.1. Description .....                                             | 4                                         |
| 2. Operator responsibility – Safety instructions .....             | 4                                         |
| 2.1. Disposal .....                                                | 6                                         |
| 2.2. EC Conformity .....                                           | 7                                         |
| 3. Technical specifications.....                                   | 9                                         |
| 3.1. Cooling water connection .....                                | 12                                        |
| 4. Safety notes for the user.....                                  | 13                                        |
| 4.1. Explanation of safety notes .....                             | 13                                        |
| 4.2. Explanation of other notes.....                               | 13                                        |
| 4.3. Safety instructions.....                                      | 13                                        |
| 5. Installation .....                                              | 17                                        |
| 5.1. Tubing.....                                                   | 19                                        |
| 6. Operating controls and functional elements .....                | <b>Fehler! Textmarke nicht definiert.</b> |
| 7. Operating procedures .....                                      | 20                                        |
| 7.1. Bath fluids .....                                             | 20                                        |
| 7.2. Power connection.....                                         | 20                                        |
| 7.3. Filling .....                                                 | 21                                        |
| 7.4. Switching on / Start - Stop .....                             | 21                                        |
| 7.5. Setting the feed pressure .....                               | 22                                        |
| 7.6. Setting the temperatures .....                                | 22                                        |
| 7.7. AUTOSTART ON / OFF .....                                      | 23                                        |
| 7.8. Remote control: activate – deactivate.....                    | 24                                        |
| 8. Safety installations.....                                       | 25                                        |
| 8.1. Excess temperature protection .....                           | 25                                        |
| 8.2. Low level protection .....                                    | 25                                        |
| 9. Troubleshooting guide / Error messages .....                    | 25                                        |
| 10. Electrical connections.....                                    | 27                                        |
| 11. Remote control .....                                           | 28                                        |
| 11.1. Setup for remote control.....                                | 28                                        |
| 11.2. Communication with a PC or a superordinated data system..... | 28                                        |
| 11.3. List of commands .....                                       | 29                                        |
| 11.4. Status messages.....                                         | 29                                        |
| 11.5. Error messages.....                                          | 30                                        |
| 12. Cleaning / repairing the unit.....                             | 31                                        |
| 12.1. JULABO Service – Online remote diagnosis .....               | 33                                        |
| 12.2. Draining .....                                               | 34                                        |
| 13. Adequate storing of operating manual .....                     | 34                                        |
| 14. Warranty conditions.....                                       | 35                                        |


## 1. Intended use

JULABO recirculating coolers have been designed for temperature application to specific fluids. The pump connections can be used for cooling applications in an external circuit at a constant temperature.



JULABO water baths are not suitable for direct temperature control of foods, semi-luxury foods and tobacco, or pharmaceutical and medical products. Direct temperature control means unprotected contact of the object with the bath medium (bath fluid).

### 1.1. Description

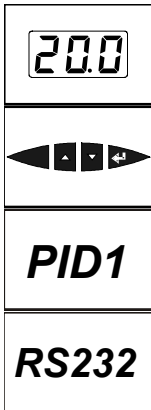

- ☑ The recirculating coolers are operated via the splash-proof keypad. The implemented microprocessor technology allows to set and to store the setpoint that can be indicated on the LED temperature display.
- ☑ The PID temperature regulation is used to withdraw heat from the bath fluid by means of the cooling machine and to automatically regulate the required need.
- ☑ Electrical connections:
  1. The serial interface RS232 allows modern process technology without additional interface.
  2. Alarm output for external alarm message.
- ☑ Manually adjustable by-pass (handwheel) to reduce the pump capacity (e. g. for glass equipment).

## 2. Operator responsibility – Safety instructions

The products of JULABO ensure safe operation when installed, operated, and maintained according to common safety regulations. This section explains the potential dangers that may arise when operating the circulator and also specifies the most important safety precautions to preclude these dangers as far as possible.

The operator is responsible for the qualification of the personnel operating the units.

- The personnel operating the units should be regularly instructed about the dangers involved with their job activities as well as measures to avert these dangers.
- Make sure all persons tasked with operating, installing, and maintaining the unit have read and understand the safety information and operating instructions.
- When using hazardous materials or materials that could become hazardous, the unit may be operated only by persons who are absolutely familiar with these materials and the unit. These persons must be fully aware of possible risks.

If you have any questions concerning the operation of your unit or the information in this manual, please contact us!

**Contact** JULABO GmbH  
Gerhard-Juchheim-Strasse 1  
77960 Seelbach / Germany

Tel. +49 7823 51-0  
Fax +49 7823 2491

[info.de@julabo.com](mailto:info.de@julabo.com)  
[www.julabo.com](http://www.julabo.com)

## Safety recommendations for the operator

- You received a product conceived for industrial use. Nevertheless, avoid strikes to the housing, vibrations, damages to the keypad foil (keys, display) or contamination.
- Make sure the product is regularly checked for proper condition. Regularly check (at least every 2 years) the proper condition of the mandatory, warning, prohibition and safety labels.
- Take care that the mains supply features a low impedance to avoid any negative affects on the instrument being operated in the same mains.
- This unit is designed for operation in a controlled electromagnetic environment. This means that transmitting devices (e.g. cellular phones) should not be used in the immediate vicinity. Magnetic radiation may influence other units with components susceptible to magnetic fields (e.g. a monitor). We recommend to keep a minimum distance of 1 m.
- Permissible ambient temperature: max. 40 °C, min. 5 °C.
- Permissible relative air humidity: 50 % (40 °C).
- Do not store in an aggressive atmosphere. Protect from contaminations.
- Do not expose to sunlight.

## Appropriate Operation

Only qualified personnel is authorized to perform configuration, installation, maintenance and repairs of the water bath.

Routine operation can also be carried out by untrained personnel who should however be instructed by trained personnel.

## Use

For the use according to the intended purpose, special material requirements have to be respected (bath fluids). Only use non-acid and non corroding materials.

Observe all warnings for the used materials (bath fluids) and the respective instructions (safety data sheets).

Only use the unit in well ventilated areas. (see page 17).

The recirculating coolers are not for use in explosive atmosphere

When using hazardous materials or materials that could become hazardous, **the operator must** affix the enclosed safety labels (**1 + 2**) to the front of the unit so they are highly visible:

|         |                                                                                     |                                                                                                                                    |
|---------|-------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------|
| 1       |  | Warning label W00: Colors: yellow, black<br>Danger area. Attention! Observe instructions.<br>(operating manual, safety data sheet) |
| 2<br>or |  | Mandatory label M018: Colors: blue, white<br>Carefully read the user information prior to beginning operation.<br><b>Scope: EU</b> |
| 2       |  | Semi S1-0701 Table A1-2 #9<br>Carefully read the user information prior to beginning operation.<br><b>Scope: USA, NAFTA</b>        |

Observe the instructions in the manuals for instruments of a different make that you connect to the circulator, particularly the corresponding safety instructions. Also observe the pin assignment of plugs and technical specifications of the products.

## 2.1. Disposal

This unit contains the refrigerant R404A, which at this time is not considered harmful to the ozone layer. However, over the long operating period of the unit, disposal rules may change. Therefore, only qualified personnel should handle the disposal.

Valid in EU countries

See the current official journal of the European Union – WEEE directive.

Directive of the European Parliament and of the Council on waste electrical and electronic equipment (WEEE).

This directive requires electrical and electronic equipment marked with a crossed-out trash can to be disposed of separately in an environmentally friendly manner.

Contact an authorized waste management company in your country.

Disposal with household waste (unsorted waste) or similar collections of municipal waste is not permitted!



## 2.2. EC Conformity

### EG-Konformitätserklärung nach EG Maschinenrichtlinie 2006/42/EG, Anhang II A EC-Declaration of Conformity to EC Machinery Directive 2006/42/EC, Annex II A

Hersteller / Manufacturer:

JULABO GmbH  
Gerhard-Juchheim-Strasse 1  
77960 Seelbach / Germany  
Tel: +49(0)7823 / 51 - 0



Hiermit erklären wir, dass das nachfolgend bezeichnete Produkt  
We hereby declare, that the following product

Produkt / Product: Umlaufkühler / Recirculating Cooler

Typ / Type: FL7006, FLW7006

Serien-Nr. / Serial-No.: siehe Typenschild / see type label

aufgrund seiner Konzipierung und Bauart in der von uns in Verkehr gebrachten Ausführung den grundlegenden Sicherheits- und Gesundheitsanforderungen den nachfolgend aufgeführten EG-Richtlinien entspricht.  
due to the design and construction, as assembled and marketed by our Company – complies with fundamental safety and health requirements according to the following EC-Directives.

**Maschinenrichtlinie 2006/42/EG; Machinery Directive 2006/42/EC**

**EMV-Richtlinie 2004/108/EG; EMC-Directive 2004/108/EC (bis zum / until 19. April 2016)**

**EMV-Richtlinie 2014/30/EU; EMC-Directive 2014/30/EU (vom / from 20. April 2016)**

**RoHS-Richtlinie 2011/65/EU; RoHS-Directive 2011/65/EU**

#### Angewandte harmonisierte Normen und techn. Spezifikationen:

The above-named product is in compliance with the following harmonized standards and technical specifications:

EN 50581 : 2012

Technische Dokumentation zur Beurteilung von Elektro- und Elektronikgeräten hinsichtlich der Beschränkung gefährlicher Stoffe  
Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances

EN ISO 12100 : 2010

Sicherheit von Maschinen - Allgemeine Gestaltungsgrundsätze - Risikobeurteilung und Risikominderung (ISO 12100:2010)  
Safety of machinery - General principles for design - Risk assessment and risk reduction (ISO 12100:2010)

EN 61010-1 : 2010

Sicherheitsbestimmungen für elektrische Mess-, Steuer-, Regel- und Laborgeräte, Teil 1: Allgemeine Anforderungen  
Safety requirements for electrical equipment for measurement, control, and laboratory use, Part 1: General requirements

EN 61010-2-010 : 2014

Sicherheitsbestimmungen für elektrische Mess-, Steuer-, Regel- und Laborgeräte, Teil 2-010: Besondere Anforderungen an Laborgeräte für das Erhitzen von Stoffen  
Safety requirements for electrical equipment for measurement, control, and laboratory use, Part 2-010: Particular requirements for laboratory equipment for the heating of materials

EN 61326-1 : 2013

Elektrische Mess-, Steuer-, Regel- und Laborgeräte- EMV-Anforderungen- Teil 1: Allgemeine Anforderungen  
Electrical equipment for measurement, control, and laboratory use - EMC requirements - Part 1: General requirements

EN 378-1 : 2008 + A2 : 2012

Kälteanlagen und Wärmepumpen – Sicherheitstechnische und umweltrelevante Anforderungen – Teil 1: Grundlegende Anforderungen  
Refrigerating systems and heat pumps - Safety and environmental requirements - Part 1: Basics requirements, definitions, classification and selection criteria

EN 378-2 : 2008 + A2 : 2012

Kälteanlagen und Wärmepumpen – Sicherheitstechnische und umweltrelevante Anforderungen – Teil 2: Konstruktion, Herstellung, Prüfung, Kennzeichnung und Dokumentation  
Refrigerating systems and heat pumps - Safety and environmental requirements - Part 2: Design, construction, testing, marking and documentation

EN 378-3 : 2008 + A1 : 2012

Kälteanlagen und Wärmepumpen – Sicherheitstechnische und umweltrelevante Anforderungen – Teil 3: Aufstellungsort und Schutz von Personen  
Refrigerating systems and heat pumps - Safety and environmental requirements - Part 3: Installation site and personal protection

EN 378-4 : 2008 + A1 : 2012

Kälteanlagen und Wärmepumpen – Sicherheitstechnische und umweltrelevante Anforderungen – Teil 4: Betrieb, Instandhaltung, Instandsetzung und Rückgewinnung  
Refrigerating systems and heat pumps - Safety and environmental requirements - Part 4: Operation, maintenance, repair and recovery

#### Bevollmächtigter für die Zusammenstellung der techn. Unterlagen:

Authorized representative in charge of administering technical documentation:

Hr. Torsten Kauschke, im Hause / on the manufacturer's premises as defined above

#### Die Konformitätserklärung wurde ausgestellt

The declaration of conformity was issued and valid of

Seelbach, 24.02.2016

M. Juchheim, Geschäftsführer / Managing Director

2016\_049\_FL(W)7006-Umlaufkühler\_d\_e.docx

**EG-Konformitätserklärung nach EG Maschinenrichtlinie 2006/42/EG, Anhang II A**  
**EC-Declaration of Conformity to EC Machinery Directive 2006/42/EC, Annex II A**

**Hersteller / Manufacturer:**

JULABO GmbH  
Gerhard-Juchheim-Strasse 1  
77960 Seelbach / Germany  
Tel: +49(0)7823 / 51 - 0



Hiermit erklären wir, dass das nachfolgend bezeichnete Produkt  
*We hereby declare, that the following product*

**Produkt / Product:** Umlaufkühler / Recirculating Cooler

**Typ / Type:** FL11006, FLW11006

**Serien-Nr. / Serial-No.:** siehe Typenschild / see type label

aufgrund seiner Konzipierung und Bauart in der von uns in Verkehr gebrachten Ausführung den grundlegenden Sicherheits- und Gesundheitsanforderungen den nachfolgend aufgeführten EG-Richtlinien entspricht.  
*due to the design and construction, as assembled and marketed by our Company – complies with fundamental safety and health requirements according to the following EC-Directives.*

**Maschinenrichtlinie 2006/42/EG; Machinery Directive 2006/42/EC**

**EMV-Richtlinie 2004/108/EG; EMC-Directive 2004/108/EC (bis zum / until 19. April 2016)**

**EMV-Richtlinie 2014/30/EU; EMC-Directive 2014/30/EU (vom / from 20. April 2016)**

**RoHS-Richtlinie 2011/65/EU; RoHS-Directive 2011/65/EU**

**Angewandte harmonisierte Normen und techn. Spezifikationen:**

*The above-named product is in compliance with the following harmonized standards and technical specifications:*

EN 50581 : 2012

Technische Dokumentation zur Beurteilung von Elektro- und Elektronikgeräten hinsichtlich der Beschränkung gefährlicher Stoffe  
*Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances*

EN ISO 12100 : 2010

Sicherheit von Maschinen - Allgemeine Gestaltungsgrundsätze - Risikobeurteilung und Risikominderung (ISO 12100:2010)  
*Safety of machinery - General principles for design - Risk assessment and risk reduction (ISO 12100:2010)*

EN 61010-1 : 2010

Sicherheitsbestimmungen für elektrische Mess-, Steuer-, Regel- und Laborgeräte, Teil 1: Allgemeine Anforderungen  
*Safety requirements for electrical equipment for measurement, control, and laboratory use, Part 1: General requirements*

EN 61010-2-010 : 2014

Sicherheitsbestimmungen für elektrische Mess-, Steuer-, Regel- und Laborgeräte, Teil 2-010: Besondere Anforderungen an Laborgeräte für das Erhitzen von Stoffen  
*Safety requirements for electrical equipment for measurement, control, and laboratory use, Part 2-010: Particular requirements for laboratory equipment for the heating of materials*

EN 61326-1 : 2013

Elektrische Mess-, Steuer-, Regel- und Laborgeräte- EMV-Anforderungen- Teil 1: Allgemeine Anforderungen  
*Electrical equipment for measurement, control, and laboratory use - EMC requirements - Part 1: General requirements*

EN 378-1 : 2008 + A2 : 2012

Kälteanlagen und Wärmepumpen – Sicherheitstechnische und umweltrelevante Anforderungen – Teil 1: Grundlegende Anforderungen  
*Refrigerating systems and heat pumps - Safety and environmental requirements - Part 1: Basics requirements, definitions, classification and selection criteria*

EN 378-2 : 2008 + A2 : 2012

Kälteanlagen und Wärmepumpen – Sicherheitstechnische und umweltrelevante Anforderungen – Teil 2: Konstruktion, Herstellung, Prüfung, Kennzeichnung und Dokumentation  
*Refrigerating systems and heat pumps - Safety and environmental requirements - Part 2: Design, construction, testing, marking and documentation*

EN 378-3 : 2008 + A1 : 2012

Kälteanlagen und Wärmepumpen – Sicherheitstechnische und umweltrelevante Anforderungen – Teil 3: Aufstellungsort und Schutz von Personen  
*Refrigerating systems and heat pumps - Safety and environmental requirements - Part 3: Installation site and personal protection*

EN 378-4 : 2008 + A1 : 2012

Kälteanlagen und Wärmepumpen – Sicherheitstechnische und umweltrelevante Anforderungen – Teil 4: Betrieb, Instandhaltung, Instandsetzung und Rückgewinnung  
*Refrigerating systems and heat pumps - Safety and environmental requirements - Part 4: Operation, maintenance, repair and recovery*

**Bevollmächtigter für die Zusammenstellung der techn. Unterlagen:**

**Authorized representative in charge of administering technical documentation:**

Hr. Torsten Kauschke, im Hause / on the manufacturer's premises as defined above

**Die Konformitätserklärung wurde ausgestellt**

*The declaration of conformity was issued and valid of*

Seelbach, 24.02.2016

  
M. Juchheim, Geschäftsführer / Managing Director

2016\_050\_FL(W)11006-Umlaufkühler\_d\_e.docx

### 3. Technical specifications

| Recirculating Cooler                   |  |             |                      | FL7006                    |  |                      | FLW7006      |  |  |
|----------------------------------------|--|-------------|----------------------|---------------------------|--|----------------------|--------------|--|--|
| Cooling                                |  |             |                      | air cooled                |  |                      | water cooled |  |  |
| Working temperature range              |  | °C          | -20 ... +40          |                           |  | -20 ... +40          |              |  |  |
| Temperature stability                  |  | °C          | ±0.5                 |                           |  |                      |              |  |  |
| Temperature selection:                 |  |             |                      | digital                   |  |                      |              |  |  |
| via key pad                            |  |             |                      | indication on LED-DISPLAY |  |                      |              |  |  |
| remote control via personal computer   |  |             |                      | indication on monitor     |  |                      |              |  |  |
| Temperature indication:                |  |             |                      | LED-DISPLAY               |  |                      |              |  |  |
| Resolution                             |  | °C          | 0.1                  |                           |  |                      |              |  |  |
| Temperature control                    |  |             |                      | PID 1                     |  |                      |              |  |  |
| Temperature sensor                     |  |             |                      | Pt 100                    |  |                      |              |  |  |
| Excess temperature protection          |  |             |                      | 85 °C - fixed value       |  |                      |              |  |  |
| Low liquid level protection            |  |             |                      | float switch              |  |                      |              |  |  |
| Cooling capacity                       |  | °C          | <u>+20   0   -10</u> |                           |  | <u>+20   0   -10</u> |              |  |  |
| Medium: Mixture water-glycol           |  | kW          | 7.0   5.1   3.0      |                           |  | 7.4   5.5   3.1      |              |  |  |
| Cooling compressor                     |  |             |                      | 1-stage                   |  |                      |              |  |  |
| Refrigerant                            |  |             |                      | R404A                     |  |                      |              |  |  |
|                                        |  |             |                      |                           |  |                      |              |  |  |
| Electrical connections:                |  |             |                      |                           |  |                      |              |  |  |
| Computer interface                     |  |             |                      | RS232                     |  |                      |              |  |  |
| Alarm output                           |  |             |                      | for external alarm signal |  |                      |              |  |  |
| Control connections                    |  | V / A       | 230 / max. 0.1       |                           |  |                      |              |  |  |
| Circulating pump:                      |  |             |                      |                           |  |                      |              |  |  |
| discharge, max.                        |  | at 0 bar    | l/min                | 60                        |  |                      | 60           |  |  |
| pressure, adjustable                   |  | at 0 Liter  | bar                  | 0.5 ... 6.0               |  |                      | 0.5 ... 6.0  |  |  |
| Feed pressure indication               |  |             | bar                  | Manometer                 |  |                      |              |  |  |
| Filling level indicator                |  |             |                      | sight glass               |  |                      |              |  |  |
| Filling volume                         |  | from ... to | liters               | 39 ... 47                 |  |                      |              |  |  |
| Dimensions (WxLxH)                     |  |             | cm                   | 78x85x148                 |  |                      |              |  |  |
| Weight                                 |  | kg          | 252                  |                           |  | 220                  |              |  |  |
| Ambient temperature range              |  | °C          | 5 ... 40             |                           |  |                      |              |  |  |
| Return flow temperature                |  | °C          | 80 max.              |                           |  |                      |              |  |  |
| Cooling water                          |  |             |                      |                           |  |                      |              |  |  |
| Flow rate at 20 °C inlet temperature   |  | l/min       | -----                |                           |  | 11.6                 |              |  |  |
| IP class according to IEC 60 529       |  |             |                      | IP 21                     |  |                      |              |  |  |
|                                        |  |             |                      |                           |  |                      |              |  |  |
| Mains power connection                 |  | V/ Hz       | 400/3PNPE/50         |                           |  | 400/3PNPE/50         |              |  |  |
| Current input at 400 V                 |  | A           | 14                   |                           |  | 14                   |              |  |  |
| Mains power connection 230 V/3PPE/60Hz |  | V/ Hz       | 230/3PPE/60          |                           |  | 230/3PPE/60          |              |  |  |
| Current input at 220 V                 |  | A           | 23                   |                           |  | 23                   |              |  |  |

All measurements have been carried out at: rated voltage and frequency,  
ambient temperature: 20 °C

| Recirculating Cooler                    |  |             | FL11006                   |             |     | FLW11006     |     |     |
|-----------------------------------------|--|-------------|---------------------------|-------------|-----|--------------|-----|-----|
| Cooling                                 |  |             | air cooled                |             |     | water cooled |     |     |
| Working temperature range               |  | °C          | -20 ... +40               |             |     | -20 ... +40  |     |     |
| Temperature stability                   |  | °C          | ±0.5                      |             |     |              |     |     |
| Temperature selection:                  |  |             | digital                   |             |     |              |     |     |
| via key pad                             |  |             | indication on LED-DISPLAY |             |     |              |     |     |
| remote control via personal computer    |  |             | indication on monitor     |             |     |              |     |     |
| Temperature indication:                 |  |             | LED-DISPLAY               |             |     |              |     |     |
| Resolution                              |  | °C          | 0.1                       |             |     |              |     |     |
| Temperature control                     |  |             | PID 1                     |             |     |              |     |     |
| Temperature sensor                      |  |             | Pt 100                    |             |     |              |     |     |
| Excess temperature protection           |  |             | 85 °C - fixed value       |             |     |              |     |     |
| Low liquid level protection             |  |             | float switch              |             |     |              |     |     |
| Cooling capacity                        |  | °C          | +20                       | 0           | -10 | +20          | 0   | -10 |
| Medium: Mixture water-glycol            |  | kW          | 11.0                      | 7.5         | 5.0 | 11.5         | 7.3 | 4.8 |
| Cooling compressor                      |  |             | 1-stage                   |             |     |              |     |     |
| Refrigerant                             |  |             | R404A                     |             |     |              |     |     |
|                                         |  |             |                           |             |     |              |     |     |
| Electrical connections:                 |  |             |                           |             |     |              |     |     |
| Computer interface                      |  |             | RS232                     |             |     |              |     |     |
| Alarm output                            |  |             | for external alarm signal |             |     |              |     |     |
| Control connections                     |  | V / A       | 230 / max. 0.1            |             |     |              |     |     |
| Circulating pump:                       |  |             |                           |             |     |              |     |     |
| discharge, max.                         |  | at 0 bar    | l/min                     | 60          |     | 60           |     |     |
| pressure, adjustable                    |  | at 0 Liter  | bar                       | 0.5 ... 6.0 |     | 0.5 ... 6.0  |     |     |
| Feed pressure indication                |  |             | bar                       | Manometer   |     |              |     |     |
| Filling level indicator                 |  |             | sight glass               |             |     |              |     |     |
| Filling volume                          |  | from ... to | liters                    | 39 ... 47   |     |              |     |     |
| Dimensions (WxLxH)                      |  |             | cm                        | 78x85x148   |     |              |     |     |
| Weight                                  |  | kg          | 248                       |             |     |              | 250 |     |
| Ambient temperature range               |  | °C          | 5 ... 40                  |             |     |              |     |     |
| Return flow temperature                 |  | °C          | 80 max.                   |             |     |              |     |     |
| Cooling water                           |  |             |                           |             |     |              |     |     |
| Flow rate at 20 °C inlet temperature    |  | l/min       | -----                     |             |     | 18.2         |     |     |
| IP class according to IEC 60 529        |  |             | IP 21                     |             |     |              |     |     |
|                                         |  |             |                           |             |     |              |     |     |
| Mains power connection 400 V/3PNPE/50Hz |  | V/ Hz       | 400/3PNPE/50              |             |     | 400/3PNPE/50 |     |     |
| Current input at 400 V                  |  | A           | 17                        |             |     | 17           |     |     |
| Mains power connection 230 V/3PPE/60Hz  |  | V/ Hz       | 230/3PPE/60               |             |     | 230/3PPE/60  |     |     |
| Current input at 230 V                  |  | A           | 27                        |             |     | 23           |     |     |

All measurements have been carried out at: rated voltage and frequency,  
ambient temperature: 20 °C

## Warning functions and safety installations

|                                         |                               |
|-----------------------------------------|-------------------------------|
| Excess temperature protection           | 85 °C - fixed value           |
| Low liquid level protection             | float switch                  |
| Alarm message                           | optical + audible (permanent) |
| Excess temperature - Warning function   | 75 °C                         |
| Overload protection                     | for compressor and pump motor |
| Classification according to DIN 12876-1 | class I                       |

## Environmental conditions according to IEC 61 010-1:

Use only indoor.

Altitude up to 2000 m - normal zero.

Ambient temperature: +5 ... +40 °C

Air humidity:

Max. rel. humidity 80 % for temperatures up to +31 °C,

linear decrease down to 50 % relative humidity at a temperature of +40 °C

Max. mains fluctuations of  $\pm 10$  % are permissible.

The unit corresponds to Class I

Overvoltage category II

Pollution degree 2



### Caution:

The unit is not for use in explosive atmosphere

Standards for interference resistance according to EN 61326-1

This unit is an ISM device classified in Group 1 (using high frequency for internal purposes) Class A (industrial and commercial range).

## Information about the used refrigerants

The **Regulation (EU) No. 517/2014 on fluorinated greenhouse gases** applies to all systems which contain fluorinated refrigerants and replaces (EC) 842/2006.

The aim of the Regulation is to protect the environment by reducing emissions of fluorinated greenhouse gases.

Among other things it regulates the emission limits, use and recovery of these substances. It also contains requirements for operators of systems which require / contain these substances to function.

Under Regulation 517/2014, the operator of a system of this nature has the following duties:

- The operator must ensure that the equipment is checked at regular intervals for leaks.
- These intervals depend on the CO<sub>2</sub> equivalent of the system. This is calculated from the refrigerant fill volume and type of refrigerant. The CO<sub>2</sub> equivalent of your system is shown on the model plate.
- The operator undertakes to have maintenance, repair, service, recovery and recycling work carried out by certified personnel who have been authorized by JULABO.
- All such work must be documented. The operator must keep records and archive them for at least five years. The records must be submitted to the relevant authority on request.

Refer to the text of the Regulation for further information.

### 3.1. Cooling water connection

Only for water cooled models - FLW:

|                                    |         |                |
|------------------------------------|---------|----------------|
| Cooling water pressure (IN / OUT ) | max.    | 6 bar          |
| Difference pressure (IN - OUT )    |         | 2 bar to 6 bar |
| Flow rate on FLW 7006              | typical | 11.6 l/min     |
| Flow rate on FLW 11006             | typical | 18.2 l/min     |
| Cooling water temperature          |         | <20 °C         |



**Notice:** **Cooling water circuit**

Risk of oil leaking from the refrigeration system (compressor) of the recirculating cooler into the cooling water in case of a fault in the cooling water circuit!  
Observe the laws and regulations of the water distribution company valid in the location where the unit is operated.

#### Recommended quality of cooling water:

|                                                                        |                                         |
|------------------------------------------------------------------------|-----------------------------------------|
| <b>pH – value</b>                                                      | <b>7.5 to 9.0</b>                       |
| Sulfate [SO <sub>4</sub> 2- ]                                          | < 100 ppm                               |
| Hydrocarbonate [HCO <sub>3</sub> - ] / Sulphate [SO <sub>4</sub> 2-]   | > 1 ppm                                 |
| Hardness [Ca <sup>2+</sup> , Mg <sup>2+</sup> ] / [HCO <sub>3</sub> -] | > 0.5 dH                                |
| Alkalinity                                                             | 60 ppm < [HCO <sub>3</sub> -] < 300 ppm |
| Conductivity                                                           | < 500 µs / cm                           |
| Chloride (CL-)                                                         | < 50 ppm                                |
| Phosphate (PO <sub>4</sub> 3-)                                         | < 2 ppm                                 |
| Ammonia (NH <sub>3</sub> )                                             | < 0.5 ppm                               |
| Free Chlorine                                                          | < 0.5 ppm                               |
| Ferri Ions (Fe <sup>3+</sup> )                                         | < 0.5 ppm                               |
| Mangano Ions (Mn <sup>2+</sup> )                                       | < 0.05 ppm                              |
| Carbon dioxide (CO <sub>2</sub> )                                      | < 10 ppm                                |
| Hydrosulfide (H <sub>2</sub> S)                                        | < 50 ppm                                |
| Content of oxygen                                                      | < 0.1 ppm                               |
| Algae growth                                                           | impermissible                           |
| Suspended solids                                                       | impermissible                           |



**Notice:**

**Danger of corrosion of heat exchanger due to unsuitable quality of cooling water.**

- Due to its high content of lime hart water is not suitable for cooling and causes calcination of the heat exchanger.
- Ferrous water or water containing ferrous particles will cause formation of rust even in heat exchangers made of stainless steel.
- Chlorous water will cause pitting corrosion in heat exchangers made of stainless steel.
- Due to its corrosive characteristics distilled and deionized water is unsuitable and will cause corrosion of the bath.
- Due to its corrosive characteristics sea water is not suitable.
- Due to its microbiological (bacteria) components which settle in the heat exchanger untreated and unpurified river water and water from cooling towers is unsuitable.
- Avoid particulate matter in cooling water.
- Avoid putrid water.

## 4. Safety notes for the user

### 4.1. Explanation of safety notes



In addition to the safety warnings listed above, warnings are posted throughout the manual. These warnings are designated by an exclamation mark inside an equilateral triangle. "Warning of a dangerous situation (Attention! Please follow the documentation)."

The danger is classified using a signal word.  
Read and follow these important instructions.



**Warning:**

Describes a possibly highly dangerous situation. If these instructions are not followed, serious injury and danger to life could result.



**Caution:**

Describes a possibly dangerous situation. If this is not avoided, slight or minor injuries could result. A warning of possible property damage may also be contained in the text.



**Notice:**

Describes a possibly harmful situation. If this is not avoided, the product or anything in its surroundings can be damaged.

### 4.2. Explanation of other notes



**Note!**

Draws attention to something special.



**Important!**

Indicates usage tips and other useful information.

### 4.3. Safety instructions

Follow the safety recommendations to prevent damage to persons or property.  
Further, the valid safety instructions for working places must be followed.



- Only connect the unit to a power socket with earthing contact (PE – protective earth)!
- The power supply plug serves as a safe disconnecting device from the line and must always be easily accessible.
- Place the instrument on an even surface on a pad made of non-inflammable material.
- Do not stay in the area below the unit.
- Make sure you read and understand all instructions and safety precautions listed in this manual before installing or operating your unit.
- Never operate the unit without bath fluid in the bath.
- Do not drain the bath fluid while it is hot or cold!  
Check the temperature of the bath fluid prior to draining (by switching the unit on for a short moment for example).
- Use suitable connecting tubing.
- Avoid sharp bends in the tubing, and maintain a sufficient distance from surrounding walls.


- Make sure that the tubing is securely attached.
- Regularly check the tubing for material defects (e.g., for cracks).
- Never operate damaged or leaking equipment.
- Always turn off the unit and disconnect the mains cable from the power source before performing any service or maintenance procedures, or before moving the unit.
- Always turn off the unit and disconnect the mains cable from the power source before cleaning the unit.
- Always empty the bath before moving the unit.
- Transport the unit with care.
- Sudden jolts or drops may cause damage in the interior of the unit.
- Observe all warning labels.
- Never remove warning labels.
- Never operate equipment with damaged mains power cables.
- Repairs are to be carried out only by qualified service personnel.




- Risk of injury for hands. Close cover carefully.

## 5. Operating controls and functional elements


Example: FL7006 Front view

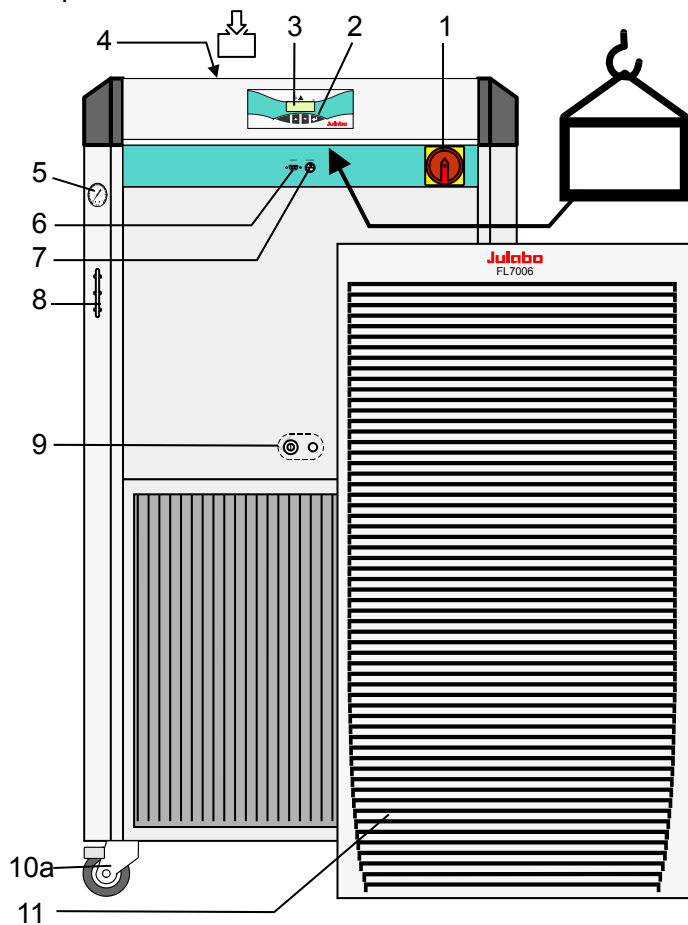

Rear view

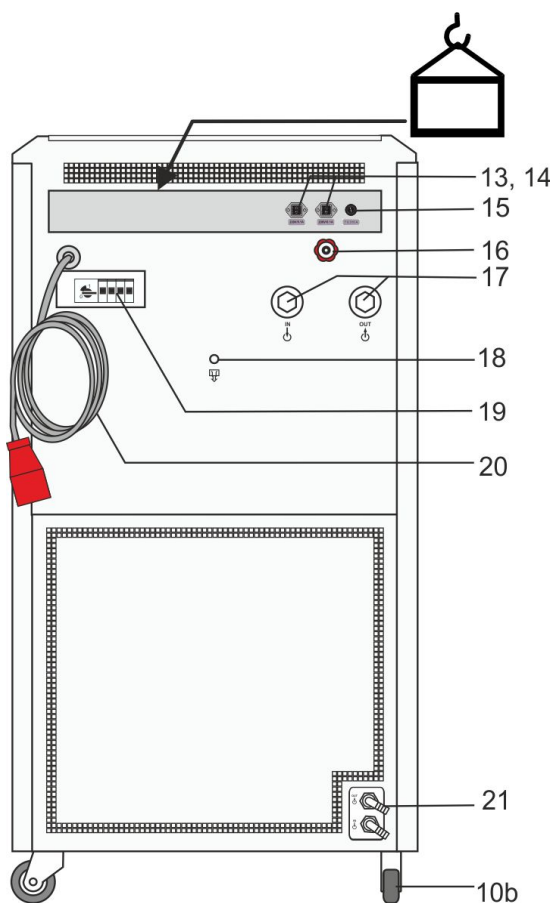

Top view



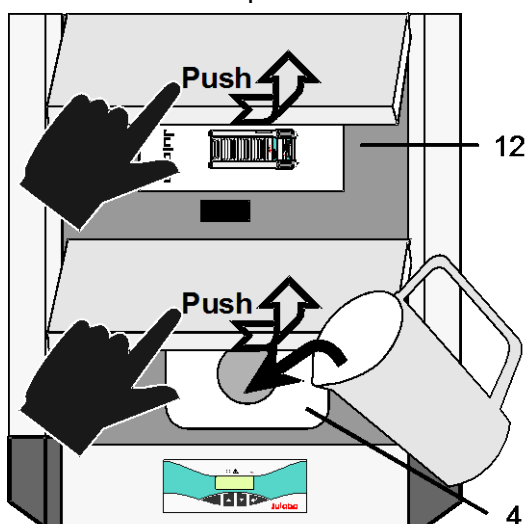



12 Protection lid for storing place of operating manual

4 Protection lid for fill in opening



Lifting device for transportation by crane

|     |                                                                                     |                                                                          |
|-----|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------|
| 1   |    | Mains power switch                                                       |
| 2.0 |    | <b>Keypad</b> , splash-water protected                                   |
| 2.1 |                                                                                     | Edit keys (set point increase or decrease)                               |
| 2.2 |                                                                                     | Enter key Store set point value / parameter                              |
| 3.0 |                                                                                     | <b>Indication</b>                                                        |
| 3.1 |    | LED temperature display                                                  |
| 3.2 |    | Control indicator – Cooling                                              |
| 3.3 |    | Control indicator – Alarm                                                |
| 4   |                                                                                     | Protection lid for fill in opening                                       |
| 5   |                                                                                     | Feed pressure indication: Manometer                                      |
| 6   |    | Interface RS232: remote control via personal computer                    |
| 7   |    | Alarm output (for external alarm signal)                                 |
| 8   |                                                                                     | Filling level indication                                                 |
| 9   |                                                                                     | Drain tap with drain port                                                |
| 10a |                                                                                     | Castor with brake (at the front)                                         |
| 10b |                                                                                     | Castor without brake (at the back)                                       |
| 11  |                                                                                     | Venting grid, removable                                                  |
| 12  |                                                                                     | Protection lid for storing place of operating manual                     |
| 13  |  | Control connection 230 V / max. 0.1 A<br>No control voltage in the “OFF” |
| 14  |                                                                                     | Control connection 230 V / max. 0.1 A<br>No control voltage in the “OFF” |
| 15  |  | Mains fuse for control connections, T 0.315 A                            |
| 16  |  | Feed pressure adjusting valve                                            |
| 17  |  | Pump connector OUT – pressure pump                                       |
|     |                                                                                     | Pump connector IN– Return<br>FL/FLW7006 G 1¼“<br>FL/FLW11006 G 1¼“       |
| 18  |  | Overflow connector                                                       |
| 19  |  | Mains circuit breakers (resettable)                                      |
|     |                                                                                     | 1 Motor protection switch for compressor motor                           |
|     |                                                                                     | 2 Mains circuit breakers (resettable) 4 A (for Electronics)              |
|     |                                                                                     | 2 Mains circuit breakers (resettable) 10 A (for Pump motor)              |
| 20  |                                                                                     | Mains power cable with plug                                              |




Only water cooled models

- |     |                         |
|-----|-------------------------|
| IN  | Cooling water inlet     |
| OUT | Cooling water outlet    |
|     | G3/4" external thread   |
|     | 12 mm inner dia. tubing |



## 6. Installation

- Place the unit on an even surface on a base made of nonflammable material. Using the castors (10a, 10b) move the unit to the intended location.  
For better stability, apply the holding breaks on the front casters (10a).
- Cooling machine, pump motor and electronics produce intrinsic heat that is dissipated via the venting openings.! Never cover these openings!
- Do not set up the unit in the immediate vicinity of heat sources and do not expose to sun light.
- Keep at least 20 cm of open space on the front and rear venting grids.
- The place of installation should be large enough and provide sufficient air ventilation to ensure the room does not warm up excessively because of the heat the instrument rejects to the environment.  
For a fault (leakage) in the refrigeration system, the standard EN 378 prescribes a certain room space to be available for each kg of refrigerant.  
> For 0.52 kg of refrigerant R-404A, 1 m<sup>3</sup> of space is required.

Rear view Example: FLW7006

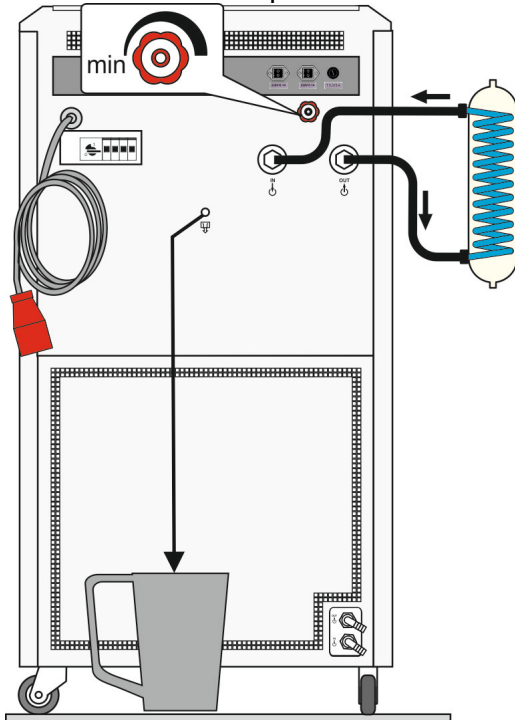

- Connect the tubings for cooling the external system to the pump connectors M16x1 for feed and return (14) on the rear of the recirculating cooler.
- Return     - Feed
- Connect a piece of tubing to the overflow connector (15) and drain into a suitable vessel, which always has to be placed lower than the exit „Overflow“.
  - Turn the adjusting valve (13) counter-clockwise to set the lowest manometric pressure.
  - Before operating the unit after transport, wait about one hour after setting it up. This will allow any oil that has accumulated laterally during transport to flow back down thus ensuring maximum cooling performance of the compressor.



- Only water cooled models - FLW:  
Ensure circulation of cooling water by connecting the tubing to cooling water inlet (IN) and outlet (OUT) on the rear (18) of the recirculating cooler.

Cooling water see page 11.

Cooling water connectors G3/4" external thread

Tubing 12 mm inner dia. tubing

IN Cooling water inlet

OUT Cooling water outlet

Even high quality heat exchangers as they are installed in our equipment can be damaged by unsuitable cooling water.

The quality of the cooling water depends on the local conditions.

The heat exchanger may become leaky due to corrosion or it may become clogged due to particulate matter



#### **Caution: Pump pressure**

- Determine and check the max. admissible pressure for the external circuit before putting the unit into operation. The max. pressure is determined by the weakest element in the circuit (e. g. glass equipment).
- Securely attach all tubing to prevent slipping.



#### **Notice:**


##### **Flood hazard!**

##### **Return flow safety device**

In case the system to be cooled is located at a higher level than the recirculating cooler, take note of bath liquid flowing back when the unit is switched off.

Should the filling volume of the bath tank not be sufficient, prevent the liquid from flowing back by using solenoid valves.

Expl. of a return flow safety device  
FLW7006

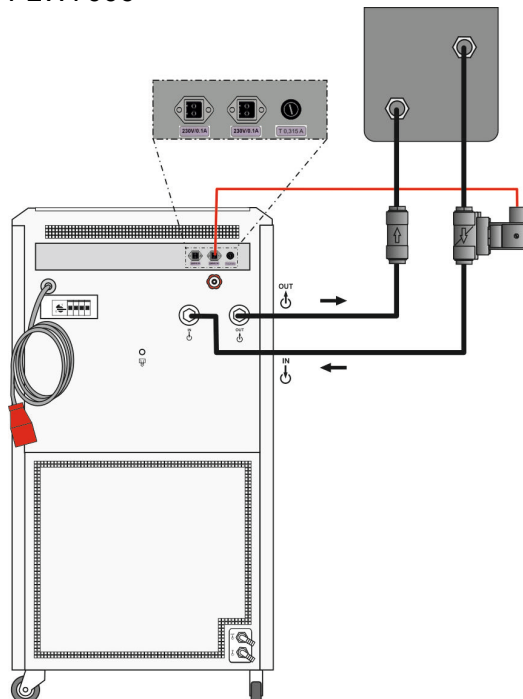

The solenoid valve set consists of

- Solenoid valve
- nonreturn valve
- Connection cable with plug

- The nonreturn valve is fitted into the feed of the cooling system.
- The solenoid valve is fitted into the return line and connected with the cable to the control connection (14).

| Suitable for     | Order text                     | Order No.  |
|------------------|--------------------------------|------------|
| FL(W) 7006/11006 | Solenoid valve set<br>G 1 1/4" | on request |

The following questions shall help to recognize possible dangers and to reduce the risks to a minimum.

- Are all tubes and electrical cables connected and installed?  
Note:  
sharp edges, hot surfaces in operation, moving machine parts, etc.
- What to do when a dangerous substance was spilled on or in the unit?  
Before starting to work, obtain information concerning the substance and determine the method of decontamination.

## 6.1. Tubing



### Caution:

- Employ suitable connecting tubing.
- Make sure that the tubing is securely attached.
- Avoid sharp bends in the tubing, and maintain a sufficient distance from surrounding walls.
- Regularly check the tubing for material defects (e.g. for cracks).
- Preventive maintenance: Replace the tubing from time to time.

### Recommended tubing:

| Order No. | Description                                          | Suitable for     |
|-----------|------------------------------------------------------|------------------|
| 8930325   | 1 m Reinforced tubing 1" inner dia. (-40 ... +120°C) | FL(W) 7006/11006 |

### Tubing insulation

|         |                                  |                                 |
|---------|----------------------------------|---------------------------------|
| 8930425 | 1 m Insulation, 35 mm inner dia. | Reinforced tubing 1" inner dia. |
|---------|----------------------------------|---------------------------------|

### Tube clamps

|         |                       |                                 |
|---------|-----------------------|---------------------------------|
| 8970484 | 2 Tube clamps, size 5 | Reinforced tubing 1" inner dia. |
|---------|-----------------------|---------------------------------|

## 7. Operating procedures

### 7.1. Bath fluids

**Caution:**

No liability for use of other bath liquids!

Please contact JULABO before using other than recommended bath fluids. JULABO takes no responsibility for damages caused by the selection of an unsuitable bath fluid

**Do not use alcohols.**

**Water:**

The quality of water depends on local conditions.

- Due to the high concentration of lime, hard water is not suitable for temperature control because it leads to calcification in the bath.
- Ferrous water can cause corrosion - even on stainless steel.
- Chloric water can cause pitting corrosion.
- Distilled and deionized water is unsuitable. Their special properties cause corrosion in the bath, even in stainless steel.

No liability for use with water. Danger of freezing at working temperatures <5 °C.

**Recommended bath fluids:**

| Bath fluids            | Temperature range |
|------------------------|-------------------|
| soft/decalcified water | 5 °C to 80 °C     |



See website for list of recommended bath fluids.

**Contact:** [www.julabo.com](http://www.julabo.com)

### 7.2. Power connection

**Caution:**

- Only connect the unit to a power socket with earthing contact (PE – protective earth)!
  - The power supply plug serves as safe disconnecting device from the line and must be always easily accessible.
  - Never operate equipment with damaged mains power cables.
  - Regularly check the mains power cables for material defects (e.g. for cracks).
- We disclaim all liability for damage caused by incorrect line voltages!


Make sure that the line voltage and frequency match the supply voltage specified on the type plate.

### 7.3. Filling



#### Notice:

Risk of injury for hands. Close cover carefully.

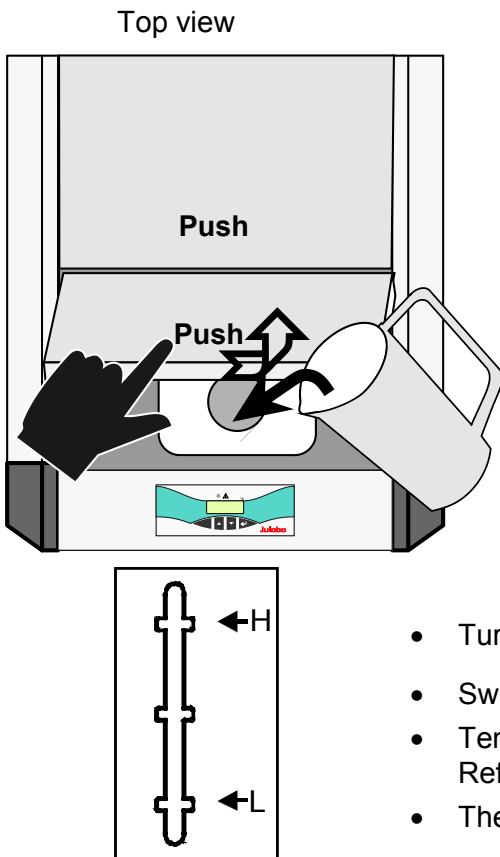

Take care that no liquid enters the interior of the circulating cooler.

- ① Connect the tubing from the external system to the pump connectors and check for leaks





Respect instructions from page 17 to page 19!

- ① Check to make sure that the drain tap (9) is closed.

- Unlock and open lid of fill in opening (4) by slightly pushing.
- Fill in tempering fluid up to marking „H“ of the filling level indicator.
- Turn the mains switch (1) on (Switching on - see page 21)
- Switch on unit. To do so press button  for approx. 4 seconds.
- Tempering fluid is pumped into the externally connected system. Refill fluid up to marking „H“.
- The recirculating cooler is ready for operation.

### 7.4. Switching on / Start - Stop



#### Switching on:


The recirculating cooler is turned on and off with the mains switch. The unit performs a self-test. All segments of the 4-digit LED temperature DISPLAY and all indicator lights will illuminate (as illustrated on the left).

Then the software version and the type of unit is indicated. Examples: (v 1.02) (FL7006)

The display "OFF" indicates the unit is ready to operate (standby mode).

- Start:** Press enter  for about 4 seconds.  
The LED temperature DISPLAY indicates the actual bath temperature.
- Stop:**
1. Press enter  for about 4 seconds.
  2. Wait until the LED display stops blinking!
  3. Turn the unit off with the mains power switch.

## 7.5. Setting the feed pressure




Set the max. permissible feed pressure (example: 2 bar) by slowly closing the adjusting valve (13) on the rear and looking at the manometer (5).

- ❗ The max. pressure is determined by the weakest element in the circuit (e. g. glass equipment).

### Fixing a leak on the adjustment valve

The stuffing box gland on the adjustment valve must be tightened if it develops a leak.

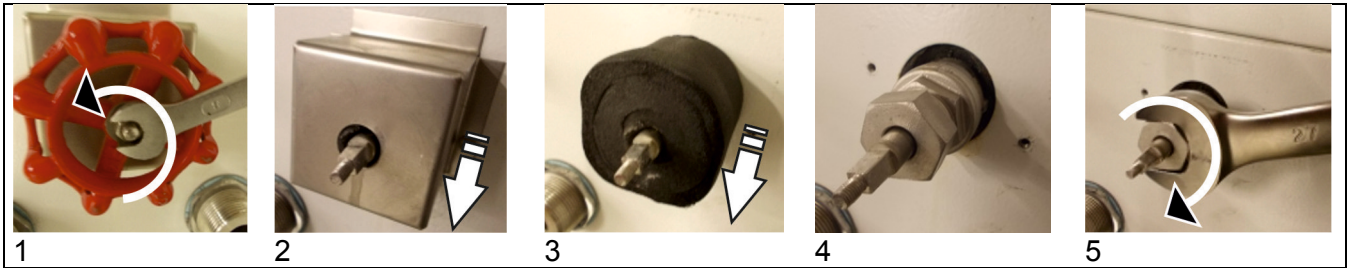

1. Undo the nut (a.f. 8) and remove the hand wheel on the adjustment valve,
2. Unscrew the stuffing box gland cover,
3. Remove the insulation,
4. + 5. Tighten the nut on the seal (a.f. 27),
6. Place the seal back over the screw connection,
7. Secure the stuffing box gland cover,
8. Attach the hand wheel to the adjustment valve and secure the nut.

The adjustment valve must turn easily after the nut has been tightened.

## 7.6. Setting the temperatures

Factory setting: 25 °C


- ❗ Setting can be carried out in the start/stop condition.

1. Press one of the keys ▼ ▲ for a short moment.  
The setpoint value instead of the actual value is indicated on the display for about 8 seconds.  
The value can now be changed.
2. Change value:  
Press ▲ to set a higher value.  
Press ▼ to set a lower value.  
Keep the keys depressed for the value to change fast.
3. Press enter ↵ to store the value.

## 7.7. AUTOSTART ON / OFF

The recirculating cooler has been configured and supplied by JULABO according to N.A.M.U.R. recommendations. This means for the start mode, that the unit must enter a safe operating state after a power failure (non-automatic start mode). This safe operating state is indicated by „OFF“ on the LED temperature display. A complete shutdown of the main functional elements such as compressor and circulating pump is effected simultaneously.

Should such a safety standard not be required, the AUTOSTART function (automatic start mode) may be activated, thus allowing the start of the circulator directly by pressing the mains power switch



Keep depressed enter  and turn on the unit with the mains power switch.

For a short while the LED DISPLAY indicates the effective start mode:

 ⇒ AUTOSTART on.  ⇒ AUTOSTART off.




### **Warning:**

For supervised or unsupervised operation with the AUTOSTART function, avoid any hazardous situation to persons or property.

The circulator does no longer conform to N.A.M.U.R. recommendations.

## 7.8. Remote control: activate – deactivate

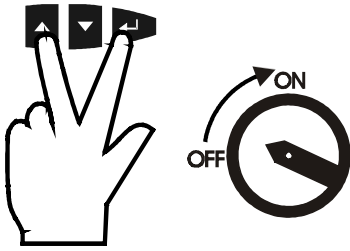

(Interface OFF)

10FF

(Interface On)

10n

u 102

FL

7006

rOFF

The recirculating cooler is to be prepared for remote control by a personal computer via the serial interface RS232.  
Set the interface item from >IOFF< to >ION<.

### Remote control: activate – deactivate:

- Switch off recirculating cooler by pressing the mains switch and wait approx. 5 seconds.
- Keep depressed the keys ▲ and enter ↵ simultaneously and turn on the unit with the mains power switch.

>I OFF< No remote control via RS232 (Factory setting)

>I On< Remote control via RS232

- ① The software version and the type of unit is indicated (see example on the left).

The display "rOFF" indicates the unit is ready to be operated via remote control.

## 8. Safety installations

### 8.1. Excess temperature protection



This safety installation is independent of the control circuit.

When the temperature of the bath fluid has reached the safety temperature (85 °C), a complete shutdown of the compressor and pump is effected.

The alarm is indicated by optical and audible signals (continuous tone) and on the LED-DISPLAY appears the error message **"Error 14"**.

### 8.2. Low level protection



This safety installation is independent of the control circuit.

If the low liquid level protection device is triggered, a complete shutdown of the compressor and circulating pump is effected.

The alarm is indicated by optical and audible signals (continuous tone) and on the LED-DISPLAY appears the error message **"Error 01"**.

❗ Turn off the unit with the mains switch, refill bath fluid and turn the unit on again!



#### Caution:

For refill always use the same bath fluid type that is already in the bath.




#### Notice:

Check the low liquid level protection device at least twice a year!

To execute a functional test, drain the liquid until the alarm for low liquid level is triggered. Refill liquid afterwards.

## 9. Troubleshooting guide / Error messages



Whenever the microprocessor electronics registers a failure, a complete

shutdown of the compressor and circulating pump is performed. The alarm light

"" illuminates and a continuous signal tone sounds.

The LED temperature display indicates the cause for the alarm in form of a code.



Press enter  to quit the audible signal.



- The recirculating cooler is operated without bath fluid, or the liquid level is insufficient.

Replenish the bath tank with the bath fluid.

- Tube breakage has occurred (insufficient filling level due to excessive bath fluid pumped out). Replace the tubing and replenish the bath tank with the bath fluid.



Cable of the working temperature sensor interrupted or short-circuited.



Error in A/D converter

E 14

The return temperature is above the switch-off value of the high temperature protection (85 °C). Check dimensioning of application.  
Use a stronger recirculating cooler if necessary.

E 51


- The motor protection switch for the compressor motor is off. Set motor protection switch to >1< . Check the fuses.
- The pressure sensor of low pressure side (evaporation pressure) is faulty, short-circuited or has a line interruption.  
Have the repair done by a specialist.

E 52

- The motor protection switch for the compressor motor is off. Set motor protection switch to >1< . Check the fuses.
- The pressure sensor of high pressure side is faulty, short-circuited or has a line interruption.  
Have the repair done by a specialist.

E 53

The suction gas temperature sensor is faulty, short-circuited or has a line interruption.  
Have the repair done by a specialist.



After eliminating the malfunction, press the mains power switch off and on again to cancel the alarm state.  
If the unit cannot be returned to operation, contact an authorized service station.

E 03

### Warning without a complete shutdown of the unit

Excess temperature warning starting at 75 °C  
The return temperature soon reaches the switch-off value of the high temperature protection (85 °C).

E 20

Cooling of the condenser is affected. (see page 31)

- Clean air-cooled condenser.
- Check the flow rate and cooling water temperature on water-cooled condenser.


If the unit cannot be returned to operation, contact an authorized JULABO service station.

### Disturbances that are not indicated.

Overload protection::      a) for cooling machine  
                                             b) for pump motor

After a short cooling interval, the unit will automatically start running.

Mains circuit breakers (resettable)



1 Motor protection switch for compressor motor

2 Mains circuit breakers (resettable) 4 A      (for electronics)

2 Mains circuit breakers (resettable) 10 A      (for pump motor)

## 10. Electrical connections

**Notice:**


Use shielded cables only.

The shield of the connecting cable is electrically connected to the plug housing.

The unit ensures safe operation if connecting cables with a maximum length of 3 m are used. The use of longer cables does not affect proper performance of the unit, however external interferences may have a negative impact on safe operation.

### RS232 serial interface


This port can be used to connect a computer with an RS232 cable for remote control of the recirculating cooler.



### Pin assignments RS232:

|       |     |                 |
|-------|-----|-----------------|
| Pin 2 | RxD | Receive Data    |
| Pin 3 | TxD | Transmit Data   |
| Pin 5 | 0 V | Signal GND      |
| Pin 7 | RTS | Request to send |
| Pin 8 | CTS | Clear to send   |

Pin 1; 4; 6, 9 Reserved - do not use!




### Control connections (13, 14)

The output voltage is applied when the unit is working for example after pressing the start/stop button. The valve is open.

Output voltage: 230 V~ / 0.1 A max

### Accessories:

| Order No. | Description                                 |
|-----------|---------------------------------------------|
| 8 980 073 | RS232 interface cable 9-pol./9-pol. , 2.5 m |
| 8 900 110 | USB interface adapter cable                 |

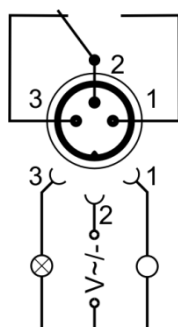

### Alarm output

Potential-free change-over contact for external alarm signal.

Pin 2 and 3 are connected in case of an alarm.


Pin 2 and 1 are connected in normal condition or mains switch "Off".

**-150 OFF -OFF** or **0000**

|                    |      |              |
|--------------------|------|--------------|
| Switching capacity | max. | 30 W / 30 VA |
| Switching voltage  | max. | 30 V~/—      |
| Switching current  | max. | 1 A          |

## 11. Remote control

### 11.1. Setup for remote control



Check the interface parameters for both interfaces (on recirculating cooler and PC) and make sure they match.

**Interface parameters are pre-determined.**

|                  |                    |
|------------------|--------------------|
| <b>Type</b>      | RS232              |
| <b>Baudrate</b>  | 4800 bauds         |
| <b>Parity</b>    | even               |
| <b>Handshake</b> | hardware handshake |

### 11.2. Communication with a PC or a superordinated data system

If the recirculating cooler is put into remote control mode the MULTI-DISPLAY (LED) will read „R -OFF-„ = REMOTE STOP. The recirculating cooler is now operated via the computer.

In general, the computer (master) sends commands to the recirculating cooler (slave). The recirculating cooler sends data (including error messages) only when the computer sends a query.



In remote control mode:

After a power interruption the order to start and all values which have to be adjusted must be resent from the personal computer via the interface. AUTOSTART is not possible.

A transfer sequence consists of:

- command out/in command
  - space (↔; Hex: 20) out/in command
  - parameter (the character separating decimals in a group is the period) out command
  - end of file (↵; Hex: 0D) out/in command
- The response (data string) after an **in** command is always followed by a line feed (LF, Hex: 0A).

#### Important times for a command transmission:

To ensure a safe data transfer, the time gap between two commands should be at least 250 ms.

The recirculating cooler automatically responds to an **in** command with a data string followed by a LF (Line Feed). The next command should only be sent after 10 ms.

The commands are divided into **in** or **out** commands.

**in** commands: asking for parameters to be displayed  
**out** commands: setting parameters



Examples:

|                                         |                          |
|-----------------------------------------|--------------------------|
| Set the working temperature to 15.5 °C: | <b>out_sp_00 ↔ 15.5↵</b> |
| Ask for the working temperature         | <b>in_sp_00↵</b>         |
| Response from the recirculating cooler: | <b>15.5↵ LF</b>          |

### 11.3. List of commands

**out commands:** Setting parameters or temperature values.

| Command     | Parameter | Response of recirculating cooler |
|-------------|-----------|----------------------------------|
| out_mode_05 | 0         | Stop the unit = R –OFF-.         |
| out_mode_05 | 1         | Start the unit.                  |
| out_sp_00   | xxx.xx    | Set working temperature          |

**in commands:** Asking for parameters or temperature values to be displayed.

| Command    | Parameter | Response of recirculating cooler                                       |
|------------|-----------|------------------------------------------------------------------------|
| version    | none      | Number of software version (V X.xx)                                    |
| status     | none      | Status message, error message (see page 29 )                           |
| in_pv_00   | none      | Actual bath temperature.                                               |
| in_sp_00   | none      | Working temperature                                                    |
| in_mode_05 | none      | Recirculating cooler in Stop/Start condition:<br>0 = Stop<br>1 = Start |

### 11.4. Status messages

| Status messages | Description                                  |
|-----------------|----------------------------------------------|
| 00 MANUAL STOP  | Recirculating cooler in „OFF“ state.         |
| 01 MANUAL START | Recirculating cooler in keypad control mode. |
| 02 REMOTE STOP  | Recirculating cooler in „r OFF“ state.       |
| 03 REMOTE START | Recirculating cooler in remote control mode. |

## 11.5. Error messages

| Error messages                                                                     | Description                                                                                                                                                                                                                                                                                                                                           |
|------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>-01 LOW LEVEL ALARM</b>                                                         | Low liquid level alarm.                                                                                                                                                                                                                                                                                                                               |
| <b>-05 WORKING SENSOR ALARM</b>                                                    | Working temperature sensor short-circuited or interrupted.                                                                                                                                                                                                                                                                                            |
| <b>-03 EXCESS TEMPERATURE WARNING</b>                                              | High temperature warning. Starting at 75 °C (no deactivation)<br>The return temperature soon reaches the switch-off value of the high temperature warning function (85 °C)                                                                                                                                                                            |
| <b>-07 I<sup>2</sup>C-BUS ERROR</b>                                                | Internal error when reading or writing the I <sup>2</sup> C bus.                                                                                                                                                                                                                                                                                      |
| <b>-08 INVALID COMMAND</b>                                                         | Invalid command.                                                                                                                                                                                                                                                                                                                                      |
| <b>-09 COMMAND NOT ALLOWED IN CURRENT OPERATING MODE</b>                           | Invalid command in current operating mode.                                                                                                                                                                                                                                                                                                            |
| <b>-10 VALUE TOO SMALL</b>                                                         | Entered value too small.                                                                                                                                                                                                                                                                                                                              |
| <b>-11 VALUE TOO LARGE</b>                                                         | Entered value too large.                                                                                                                                                                                                                                                                                                                              |
| <b>-12 TEMPERATURE MEASUREMENT ALARM</b>                                           | Error in A/D converter.                                                                                                                                                                                                                                                                                                                               |
| <b>-14 EXCESS TEMPERATURE PROTECTOR ALARM</b>                                      | The return temperature is above the switch-off value of the high temperature warning function of 85 °C.<br>Check dimensioning of application.<br>Use a stronger recirculating cooler if necessary.                                                                                                                                                    |
| <b>-20 WARNING: CLEAN CONDENSOR OR CHECK COOLING WATER CIRCUIT OF REFRIGERATOR</b> | Cooling of the condenser is affected. Clean air-cooled condenser.<br>Check the flow rate and cooling water temperature on water-cooled condenser.                                                                                                                                                                                                     |
| <b>-51 PRESSURE SENSOR ALARM LOW PRESSURE SIDE</b>                                 | <ul style="list-style-type: none"><li>• The motor protection switch for the compressor motor is off. Set motor protection switch to &gt;1&lt; . Check the fuses.</li><li>• The pressure sensor of low pressure side (evaporation pressure) is faulty, short-circuited or has a line interruption.<br/>Have the repair done by a specialist.</li></ul> |
| <b>-52 PRESSURE SENSOR ALARM HIGH PRESSURE SIDE</b>                                | <ul style="list-style-type: none"><li>• The motor protection switch for the compressor motor is off. Set motor protection switch to &gt;1&lt; . Check the fuses.</li><li>• The pressure sensor of high pressure side is faulty, short-circuited or has a line interruption.<br/>Have the repair done by a specialist.</li></ul>                       |
| <b>-53 SUCTION GAS TEMPERATURE SENSOR ALARM</b>                                    | The suction gas temperature sensor is faulty, short-circuited or has a line interruption.<br>Have the repair done by a specialist.                                                                                                                                                                                                                    |

## 12. Cleaning / repairing the unit



### Caution:

Always turn off the unit and disconnect the mains cable from the power source before cleaning the unit.  
Prevent humidity from entering into the circulator.  
Electrical connections and any other work must be performed by qualified personnel only.



### Notice:


Risk of injury for hands when mounting the venting grid.

### Maintaining the cooling performance

#### Air cooled models = FL

To maintain the full cooling performance, clean the condenser from time to time.


- Switch off the unit, disconnect mains power cable.
- Hold the venting grid, pull out and remove.
- Clean the ribbed condenser with a vacuum cleaner.
- Replace the venting grid.
- Switch on the unit.

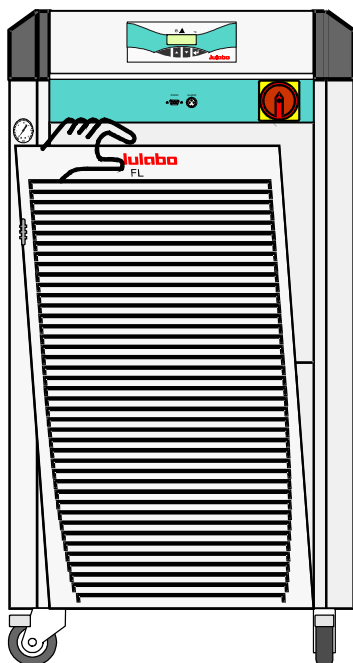

#### Water cooled models = FLW

In order to maintain a good condition of the cooling compressor, the sieve in the cooling water input should be cleaned in regular intervals.

- Switch the unit off, disconnect the power plug.
- Interrupt the cooling water input.
- Disconnect the tubing from the nozzle „IN“ and take out the dirty sieve.
- Clean the sieve.
- Put in the sieve and reconnect the tubing.
- Open the cooling water input.
- Take care the tubing connection is not leaking.
- The unit is ready to operate again.

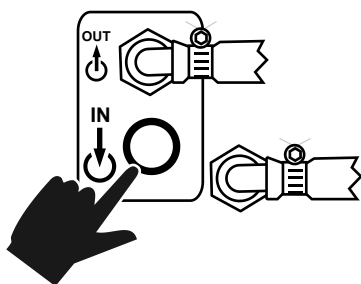

**Cleaning:**

Clean the outside of the unit using a wet cloth and low surface tension water.

The recirculating cooler is designed for continuous operation under normal conditions. Periodic maintenance is not required.

The tank should be filled only with a bath fluid recommended by JULABO. To avoid contamination, it is essential to change the bath fluid from time to time.

**Repairs:**

Before asking for a service technician or returning a JULABO instrument for repair, please contact an authorized JULABO service station.

When returning the unit:

- Clean the unit in order to avoid any harm to the service personnel
- Attach a short fault description.
- When returning a unit, take care of careful and adequate packing.
- During transport the unit has to stand upright. Mark the packing correspondingly.
- JULABO is not responsible for damages that might occur from insufficient packing.




JULABO reserves the right to carry out technical modifications with repairs for providing improved performance of a unit.

## 12.1. JULABO Service – Online remote diagnosis

JULABO circulators of the HighTech series are equipped with a black box. This box is implemented in the controller and records all significant data for the last 30 minutes.

In case of a failure, this data can be read out from the unit by using special software. This software is available as a **free** download from [www.julabo.com\EasyBlackBox](http://www.julabo.com\EasyBlackBox).

- Installation is easy and is performed step by step. Please observe the instructions.
- Data read-out is possible in the conditions “OFF”, “R OFF” or “ALARM”.
- Connect the circulator to the computer using an interface cable.
- Start the EasyBlackBox program.  
The program asks for the port used (COM1, ..... ) and the baud rate of the unit.  
You do not have this information on hand? Simply try it out!  
The program continues to send the request until the correct settings are made.

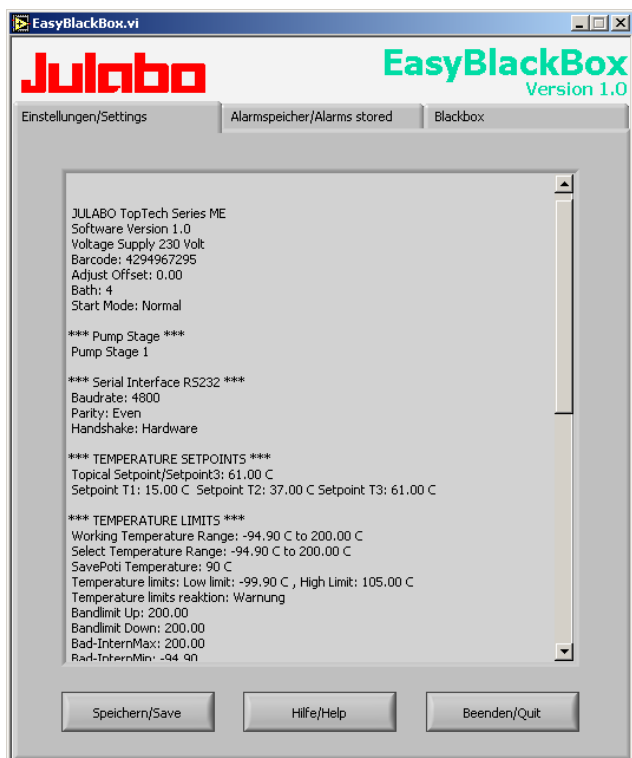

- Data is read out and shown on the monitor divided in the sections  
>Einstellungen/Settings<,  
>Alarmspeicher/Alarms stored<,  
>Blackbox<  
  
← see example
- After pressing >Speichern/Save< a text file is compiled. The program proposes a filename - >C:\model description and barcode no.<. Modifications are possible.
- E-mail this file to [service.de@julabo.com](mailto:service.de@julabo.com), JULABO's service department. JULABO is thus able to provide rapid support.



## 12.2. Draining

**Notice:**

Store and dispose the used bath fluid according to the laws for environmental protection.



Risk of injury for hands when mounting the venting grid.

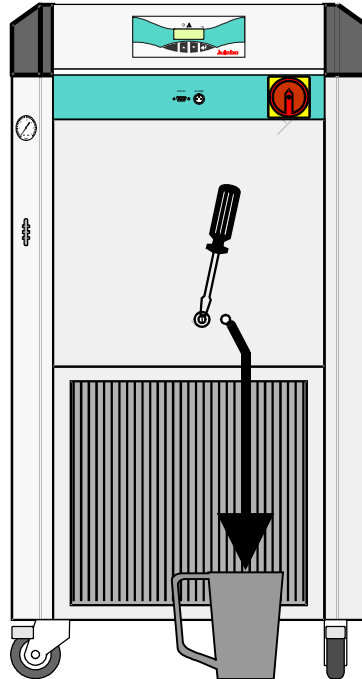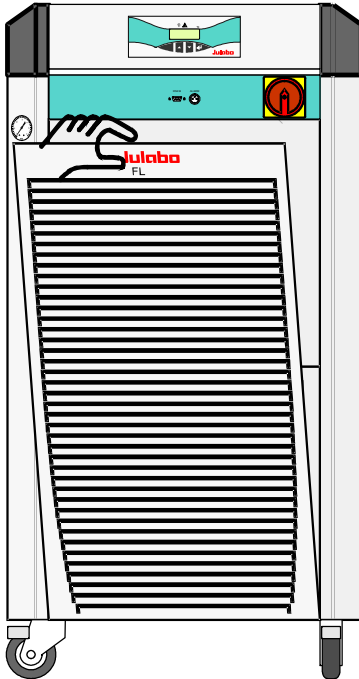

- Turn off the unit and disconnect the mains cable from the power source.
- Hold the venting grid, pull out and remove.
- Slide a short piece of tube onto the drain port and hold it into a pail.
- Open the drain tap and empty the unit completely.
- Close the drain tap and replace the venting grid.

## 13. Adequate storing of operating manual

Store the operating manual at the foreseen place at the unit and lock it by means of the protection lid (18).

## 14. Warranty conditions

JULABO GmbH warrants its products against defects in material or in workmanship, when used under appropriate conditions and in accordance with appropriate operating instructions

**for a period of ONE YEAR.**

**Extension of the warranty period – free of charge**



With the '1PLUS warranty' the user receives a free of charge extension to the warranty of up to 24 months, limited to a maximum of 10 000 working hours.

To apply for this extended warranty the user must register the unit on the JULABO web site [www.julabo.com](http://www.julabo.com), indicating the serial no. The extended warranty will apply from the date of JULABO GmbH's original invoice.

JULABO GmbH reserves the right to decide the validity of any warranty claim. In case of faults arising either due to faulty materials or workmanship, parts will be repaired or replaced free of charge, or a new replacement unit will be supplied.

Any other compensation claims are excluded from this guarantee.