

☐

I'm not robot


reCAPTCHA


I am not robot!

Sysmex xn 2100 operator

Sysmex xn-2000 operators manual. Sysmex xn operators manual. Sysmex operator's manual.

1. Ruzicka K, Veitl M, Thalhammer-Scherrer R, et al. The new hematology analyzer Sysmex XE-2100: performance evaluation of a novel white blood cell differential technology. Arch Pathol Lab Med 2001;125:391-396. [PubMed] [Google Scholar]2. Briggs C, Harrison P, Grant D, et al. New quantitative parameters on a recently introduced automated blood cell counter-the XE 2100. Clin Lab Haematol 2000;22:345-350. [PubMed] [Google Scholar]3.

Arch Pathol Lab Med 2001;125:391-396. [PubMed] [Google Scholar]2. Briggs C, Harrison P, Grant D, et al. New quantitative parameters on a recently introduced automated blood cell counter-the XE 2100. Clin Lab Haematol 2000;22:345-350. [PubMed] [Google Scholar]3. Schwartz D. Méthode statistique à l'usage des médecins et des biologistes. Paris: Flammarion Médecine Science; 1986; p 307.4. England JM, Rowan RM, Van Assendelft OW, et al. Protocol for evaluation of automated blood cell counters. International Committee for Standardization in Haematology (ICSH). Clin Lab Haematol 1984;6:69-84. [PubMed] [Google Scholar]5.

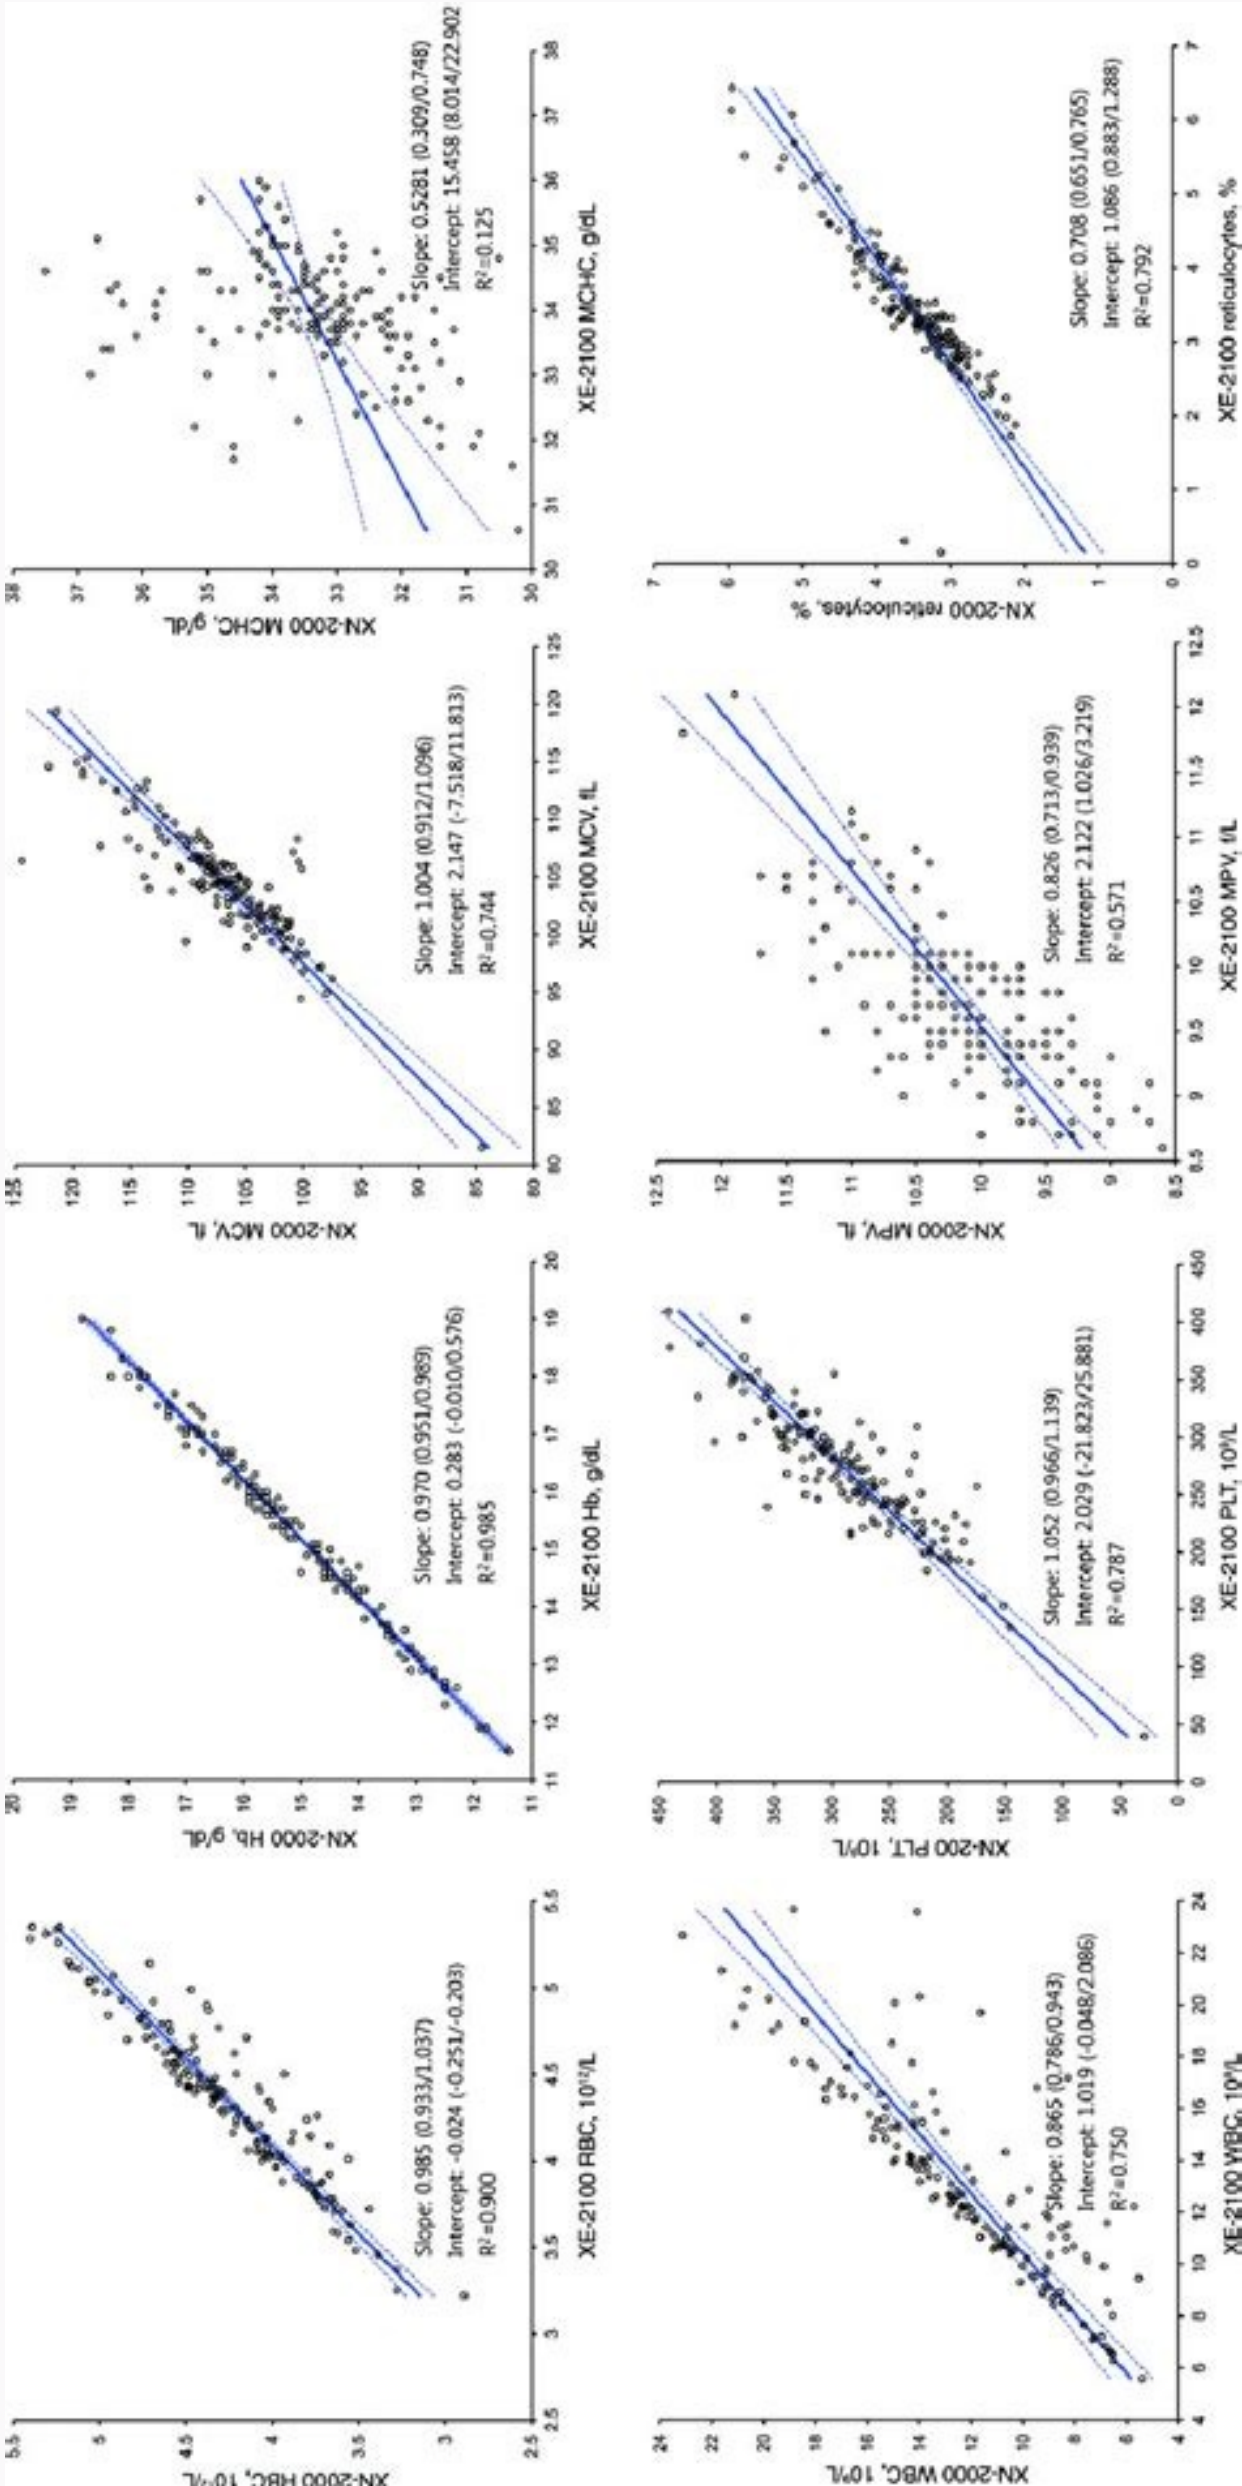

1. Ruzicka K, Veitl M, Thalhammer-Scherrer R, et al. The new hematology analyzer Sysmex XE-2100: performance evaluation of a novel white blood cell differential technology. Arch Pathol Lab Med 2001;125:391-396. [PubMed] [Google Scholar]2. Briggs C, Harrison P, Grant D, et al. New quantitative parameters on a recently introduced automated blood cell counter-the XE 2100. Clin Lab Haematol 2000;22:345-350. [PubMed] [Google Scholar]3. Schwartz D. Méthode statistique à l'usage des médecins et des biologistes. Paris: Flammarion Médecine Science; 1986; p 307.4. England JM, Rowan RM, Van Assendelft OW, et al. Protocol for evaluation of automated blood cell counters. International Committee for Standardization in Haematology (ICSH). Clin Lab Haematol 1984;6:69-84. [PubMed] [Google Scholar]5. Ferrero-Vacher C, Maerfeld K, Fraye M, et al. Évaluation du Cell-Dyn 4000® Abbott automate d'hématologie. Rev Fr Lab 2002;340:53-64. [Google Scholar]6. Ollier L, Maerfeld K, Ferrero-Vacher C, et al. Évaluation de l'automate d'hématologie Sysmex SE 9500® . Rev Fr Lab 2001;333:33-42. [Google Scholar]7. Ferrero-Vacher C, Sudaka I, Jambou D, et al. Evaluation of the ABX Cobas Vega automated hematology analyzer and comparison with the Coulter STKS. Hematol Cell Ther 1997;39:149-158. [PubMed] [Google Scholar]8. Maerfeld K. Évaluation comparative des automates haut de gamme d'hématologie au Centre Hospitalier Universitaire de Nice. Ph.D. thesis, University of Nice, Nice, France, 1999.9. Erwa W, Bauer FR, Etschmaier R, et al. Analysis of aged samples with the Abbott CD4000 hematology analyzer. Eur J Lab Med 1998;6:4-15. [Google Scholar]10. Sandhaus LM, Osei ES, Agrawal NN, et al. Platelet counting by the Coulter LH 750, Sysmex XE 2100, and Advia 120: a comparative analysis using the RBC/platelet ratio reference method. Am J Clin Pathol 2002;118:235-241. [PubMed] [Google Scholar] ForumsDocumentsVideosNews