Teledyne DALSA Shad-o-Scan 3001/4501

Detector User Manual

GigE models



Sept 15, 2020
www.TeledyneDALSA.com

© 2020 Teledyne DALSA. All information provided in this manual is believed to be accurate and reliable. No responsibility is assumed by Teledyne DALSA for its use. Teledyne DALSA reserves the right to make changes to this information without notice. Reproduction of this manual in whole or in part, by any means, is prohibited without prior permission having been obtained from Teledyne DALSA.

About Teledyne DALSA

Teledyne DALSA is an international high performance semiconductor and electronics company that designs, develops, manufactures, and markets digital imaging products and solutions, in addition to providing semiconductor products and services. Teledyne DALSA's core competencies are in specialized integrated circuit and electronics technology, software, and highly engineered semiconductor wafer processing. Products and services include image sensor components; electronic digital cameras; X-ray detectors; vision processors; image processing software; and semiconductor wafer foundry services for use in MEMS, high-voltage semiconductors, image sensors and mixed-signal CMOS circuits.

Contact Information

Please feel free to contact the global Teledyne DALSA sales office for ordering, to obtain more detailed information or in case you encounter any problem operating the detector:

Teledyne DALSA – Rad-icon Imaging
765 Sycamore Drive
Milpitas, CA 95035
USA
Tel: +1 408 736 6000
Fax: +1 408 736 6001
E-mail: sales.rad-icon@teledyne.com
Website: http://www.teledynedalsa.com/ndt

Contents

System Precautions and Safety 4
Safety Information 4
EMC compliance 5
System precautions 6
Detector Maintenance 7
The Shad-o-Scan Detector 9
Detector Highlights 9
Setting up the Detector 10
Detector Connectors and Cables 10
Setting up the Detector 14
Network Interface Card 14
Connect Trigger Cable 14
Connect Ethernet Cable 14
Connect Power Cable 14
Status Light 14
Software installation 15
Operating Systems Support 15
Obtain software 15
Sapera LT and CamExpert Installation 15
GigE Vision framework for Sapera LT installation 15
Optimizing Settings 16
Connecting 19
Quick Test with CamExpert 20
Acquiring Images 21
Operational reference 22
Using CamExpert with the Shad-o-Scan Detector 22
Camera Information 25
Camera Configuration Selection Dialog 27
Camera (Detector) Power-up Configuration 27
User Set Configuration 27
Sensor Control 28
Read-Out Mode 29
Trigger Mode 31
Image Format Control 33
Image Processing Control 34
Firmware Update 47
Mechanical Interface 50
Mechanical Dimensions 50
Appendix A 52
Revision History 52

1

System Precautions and Safety

Safety Information

Definitions

User of the products as described in this manual is the Original Equipment Manufacturer (OEM) that is developing and producing an X-ray imaging device (or 'modality'), using the product as an component to capture image information;

End-User of the products as described in this manual is the professional operating the OEM equipment to perform a diagnostic imaging routine;

Intended Use

The products as described in this manual are components that are used enclosed inside a User's system to capture images in X-ray modalities. Typical applications include, but are not limited to, Non-Destructive Testing, Electronics Inspection and Computed Tomography (CT).

Installation Warning

The User is responsible for the safe and prudent installation of the detector in their system. All X-ray sources and controls, shielding, personnel safety monitoring devices, and personnel safety precautions and training involved in the use of this equipment are the responsibility of the User and/or the End-User.

Safety Statement

The general safety precautions that follow must be observed during all phases of installation, operation, service, repair and disposal of this system. Failure to comply with these precautions, or with specific warnings noted in this manual, violates the safety standards of design, manufacture and the intended used of this system. Teledyne DALSA assumes no responsibility for the user's failure to comply with these requirements.



Warning: The product, when installed, is subject to exposure from X-rays during operation.

To ensure personnel safety, it is necessary that a radiation meter will be used to check for radiation leakage after installation of the digital camera in the end users system.

Teledyne DALSA assumes no responsibility for proper installation of the detector, installation of X-ray shielding, X-ray shield enclosure testing, or safe and prudent

operation of the camera system in the End-user's installation. It is the Users and End-users responsibility to ensure that local and federal guidelines regarding the installation and operation of X-ray sources are followed.

The power requirements of the product, especially the voltage specifications, must be strictly adhered to or warranty will be void.

No User Serviceable Components

There are no components in this system which need to be replaced, modified, or adjusted by the end user. Please contact Teledyne DALSA Support for assistance if needed.



Safety Warning: Tampering with this product voids the warranty and may degrade the detectors image quality, resulting in a possibly unsafe condition for (End-)Users.

The system has been designed to minimize the amount of interference it may generate in an installation. This equipment generates and can radiate radio frequency energy and, if not installed and operated in accordance with the instructions, may cause harmful interference to other devices in the area.

Stacking

Teledyne DALSA does not recommend that the user stack the product or use it in adjacent to other equipment. If this arrangement is unavoidable, then the (End-)user must ensure that there is adequate airflow around the detector and that normal operation conditions are maintained.

Disposal of Product

The detector contains lead and no batteries. Dispose the unit in accordance with local regulatory guidelines.

General safety instructions

- Read and follow the instructions before using the detector to ensure safe and proper use.
- Wear an ESD wrist strap, ESD clothes, or ESD gloves when installing or maintaining the detector.
- Do not install if visible damages are observed on the detector. Inspect shipping containers for any signs of damage and contact Teledyne DALSA for assistance.
- Lack of calibration can result in a lower image quality. Periodical check is necessary to ensure that the detector meets the requirements of targeted application.



EMC compliance

To ensure EMC compliance, follow these specific guidelines:

- Ensure that all cable shields have a 360° electrical connection to the connector.
- Tightly fasten and secure all connectors.

Warning



- The detector can influence the performance of very sensitive equipment.
- Strong EMC disturbances can influence the detectors performance.

System precautions

The following are precautions that must be taken in order to prevent possible damage to your Teledyne DALSA Detector:

Warning:

The use of accessories, power supplies and cables other than those specified, with the exception of cables sold by Teledyne DALSA as replacement parts, may result in increased emission or decreased immunity of the Shad-o-Scan 3001/4501 Detector.

Static precautions

Observe proper ESD/static control procedures when handling system components. The use of properly grounded wrist strap is highly recommended.





Installation Precautions

Never connect or disconnect cables while power to the detector is on. Damage to the detector electronics might occur if the cables are connected and/or disconnected while the detectors power is on.

Service by Qualified Personnel Only

This equipment is to be installed by a qualified technician only. The system can only be used in conjunction with a properly installed X-ray source with the appropriate shielding and a properly configured computer workstation that meets the minimum system requirements discussed later in this manual.

Environmental Specifications

Temperature - Operating - Transport & Storage	 +10..+40 °C -10..+55 °C
Humidity (non-condensing) - Operating - Transport & Storage	 10%...80% 10%...80%
Shock	25G (6ms)
Vibration	1G (10-150Hz)
IP Class	IP69K

Note: For transport and storage, the standard product packaging is assumed to be in place which includes a sealed anti-static shield bag.

Regulatory Compliance

The Shad-o-Scan has been designed and manufactured in accordance with the applicable clauses of the international standards and legislations.

- EN 61000-6-3: Electromagnetic compatibility (EMC) – Generic standards. Emission standard for residential, commercial and light-industrial environments
- IEC/EN 61000-6-2: Electromagnetic compatibility (EMC) – Generic standards. Immunity standard for industrial environments
- EN 50581/EN IEC 63000: Technical documentations for the assessment of electrical and electronic products with respect to the restriction of hazardous substances

Detector Maintenance

Before performing any of the following operations, make sure that the power to the detector is switched OFF.

Protecting the Detector Front Cover

The front cover of the detector and should be treated with care, as scratches or debris in this area may produce artifacts in the X-ray image.

Cleaning the Detector Body and Front Cover

The detector body and front cover can be cleaned with a mild, non-abrasive cleanser such as isopropyl alcohol. Place a small amount of cleanser on a soft cloth and rub gently over the detector body surface. Wipe off with a clean soft cloth. Do not use any harsh cleansers or solvents that may damage the paint or other finishes on the detector.

In the event of detector exposure to bio-hazardous materials, proper cleaning procedures should be undertaken prior to removal or maintenance of the detector.

Calibration

To have the best image performance, the raw image data generated by the detector should be corrected at the host by using a flat field (offset and gain) correction. As the offset (dark) calibration signal depends (amongst others) on ambient temperature conditions of the detector, it is commonly accepted good practice to generate these calibration images frequently at times that the X-ray source is switched off. It is recommended to re-calibrate the gain correction image at least once per year, or whenever the X-ray tube is exchanged or anything changes in the X-ray imaging geometry (e.g. the distance between the X-ray source and the detector).

The detector can contain deviating pixels. To have the best possible image quality it is advised to perform a defect pixel correction in the host system. It is recommended to create a defect pixel calibration map at least once every year, or more frequently in case of heavy use.

To verify if the detector still operates according specification it is advised to measure on regular base the following performance parameters of the detector: dark reference, noise performance, flatfield reference, saturation dose and MTF performance.

Recycling

EU Waste Electrical and Electronic Equipment (WEEE) Directive



The European Union (EU) implemented the EU WEEE Directive 2012/19/EU requiring producers of electrical and electronic equipment (EEE) to manage and finance the collection, re-use and recycling of the products that producers placed on the EU market after 13 August 2005. The EU Commission adopted the Implementing Regulation (EU) 2019/290 establishing the format for registration and reporting of producers of EEE to the register. The goal of this directive is to minimize the volume of EEE waste disposal and to encourage re-use and recycling at the end of life.

The WEEE symbol on the product indicates that the product cannot be disposed of with other household or municipal waste. Teledyne DALSA has labeled its products with the WEEE symbol to alert the customers that products bearing this label should not be disposed of in the landfill.

It is our customers' responsibility to dispose of their waste equipment separately from the municipal waste stream. The correct disposal of your equipment will help conserve the natural resources and ensure that the equipment is recycled in a manner that protects the environment and human health.

2

The Shad-o-Scan Detector

A full description of the features and functional specification of the Shad-o-Scan 3001 /4501 detector can be found in the latest product specification or datasheet. Please contact sales.rad-icon@TeledyneDALSA.com or visit www.TeledyneDALSA.com/ndt/ for information on how to obtain the latest datasheet or other product documentation.

Detector Highlights

Key Features

- Latest generation CMOS technology (6th generation) enables even lower noise and power consumption
- Unmatched image quality at low doses, best-in-class DQE at all doses
- 3072 x 64 pixel resolution, 99 um pixel pitch, active area 304 mm x 6.4 mm
- 4608 x 64 pixel resolution, 99 um pixel pitch, active area 456 mm x 6.4 mm
- 14-bit A/D conversion
- No measureable image lag
- Up to 1000 frames per second at full resolution, 14 bit pixel depth
- 5GigE data interface
- Gadox scintillator

Programmability

- Exposure time
- Read-out mode
- Trigger modes


3

Setting up the Detector

Detector Connectors and Cables

This detector uses the following connectors.

- An RJ-45 connector for Gigabit Ethernet signals, data signals
    - CAT6 Ethernet cable
- One 2-pin Lemo connector for power
    - Lemo EXG.0B.302.HLN
    - Mating connector:
        straight type: FGG.0B.302.CLAD52
- One 4-pin Lemo connector for triggering
    - Lemo EXG.0B.304.HLN
    - Mating connectors:
        straight type: FGG.0B.304.CLAD52

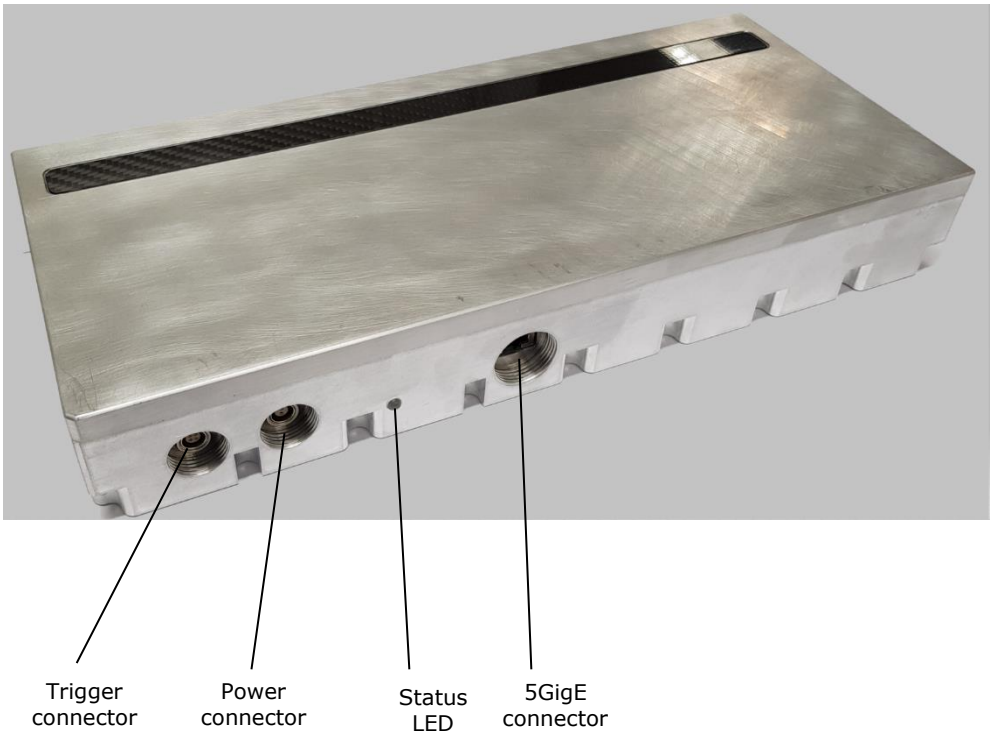

Ethernet Connector

Ethernet Connection LED

Steady orange indicates that an Ethernet connection is successfully established.

Data Transmission LED


Flashing green indicates that the detector is transmitting or receiving data.

Detector Status LED

The detector is equipped with an orange/green LED used to display the status of the detector's operation. The table below summarizes the operating states of the detector and the corresponding LED states.

	Color Of Status LED	Meaning
1	Orange	Power applied, Standby mode
2	Green	Detector is operational
3	Off	No power

Power Connector

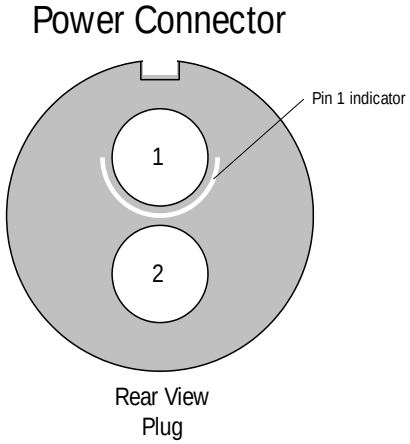

	Description
1	Supply voltage (+11-16V / 20W)
2	Ground
	Shielding (chassis)

The detector requires a single voltage input (+11-16V / 20W). There is a protection for misconnection, via a resettable fuse. When the fuse has been activated (isolating), power

cycling will return it to conductive state again thus restoring normal operation (assuming power has been properly applied).


WARNING: When setting up the detector power supplies follow these guidelines:


- Apply the appropriate voltages.
- Keep leads as short as possible in order to reduce voltage drop. The voltage level at the product power connector should be within the range mentioned in the datasheet.
- Use high-quality linear supplies of SELV type and/or EN 60601-1 compliant.

Note: If your power supply does not meet these requirements, the detector performance specifications cannot be guaranteed.

Trigger Connector

The trigger circuitry inside the detector is shown in the figure below.

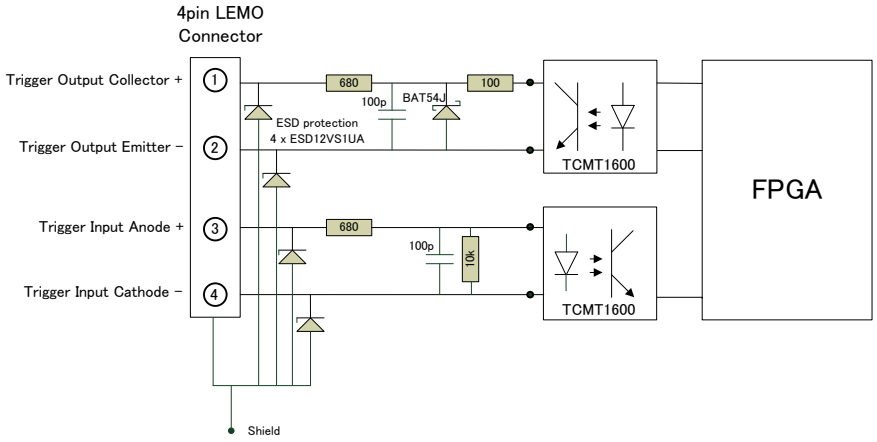

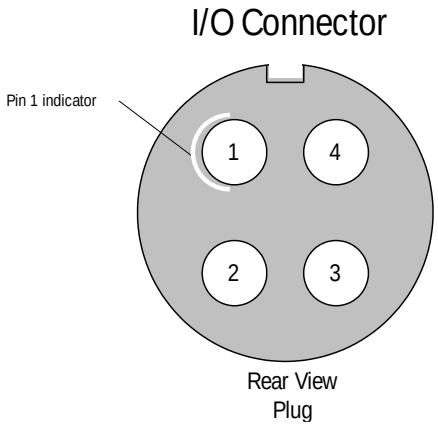

		Description
1	Out	optocoupler collector with 680R +100R series resistor (note 1)
2	Out	optocoupler emitter
3	In	optocoupler anode with 680R series resistor (note 2)
4	In	optocoupler cathode
		Shielding (chassis)

Note 1: maximum voltage across collector and emitter is 70V. Maximum reverse voltage (between emitter and collector) is 6V.
Note 2: maximum reverse voltage across cathode and anode is 6V.

Setting up the Detector

Network Interface Card

A Network Interface Card (NIC) is required to acquire images and control the Shad-o-Scan detector. A NIC with Jumbo packet support up to 9014 bytes is required to receive streaming video, preferably with a PCI Express slot.

Teledyne DALSA advises to use the 5G adapter Network Interface Card (NIC) which is a low cost but high performance and reliable adapter with a PCI Express slot.

Make sure that the latest driver of the NIC manufacturer is installed. We advise to use a 64-bit operating systems as the NIC drivers are better maintained.

Due to the high bandwidth used by the detector we strongly advise to have a direct connection from the NIC to the detector.

Connect Trigger Cable

Connect the trigger cable to the detector when the Trigger Mode of the detector is set to Trigger or Snapshot.

Connect Ethernet Cable

Connect the CAT-6 Ethernet cable from the detector to the computer Ethernet jack. Secure the RJ-45 connector to the detector.

Connect Power Cable

Connect a power cable from the detector to a power supply with a supply voltage between 11-16V and capable of delivery 20W.

Status Light

In normal operation the status light is green.

The status light is orange when the detector is in standby.

When the detector is connected to a host system it will be recognized in approximately 30 to 60 seconds.

Software installation

Operating Systems Support

The current released GigE Vision framework supports up to Windows 10.

For Linux the Teledyne DALSA GigE Vision Application Programmers Interface (API) for Linux is available.

For additional support please contact our support team for the software and the latest status.

Obtain software

Website

Visit the Teledyne DALSA website to download the latest free version of the Sapera LT SDK, including the CamExpert image viewer:

http://www.teledynedalsa.com/imaging/products/software/sapera/lt/download/

The download is free after filling out the on-line registration form. Make sure to select "Full SDK" as your download option.

Sapera LT and CamExpert Installation

A link to download the software will be emailed to you after submitting the application. Complete the download process and run the installation file (e.g. "SaperaLT80xSDKSetup.exe").

CamExpert is an image viewer designed to evaluate your detector. The Sapera SDK is a set of development tools and documentation for creating your own software for interfacing to the product. Please download the appropriate materials and follow the instructions that are part of that download.

The Sapera SDK installation also contains a large number of helpful example projects to help you get started with integration the detector into your own application software. For additional examples specific to the Shad-o-Scan 3001/4501 detector please contact our support team at the contact info listed on page 2 of this manual.

GigE Vision framework for Sapera LT installation

The GigE Vision framework installs the GigE Vision Module for Sapera and includes the Network Imaging package which is required to access a GigE Vision detector.

Refer to the "GigE Vision Module for Sapera" user manual and "Network Imaging Module for Sapera LT" user manual which are included in the installation.

Optimizing Settings


The performance of the 5Gigabit Ethernet connection on the host computer generally can be improved by adjusting some settings in the NIC. The below advices refer to the Aquantia AQtion 5Gbit NIC adaptor. For a more detailed explanation please refer to “Network Optimization Guide (PDF)” and “Network Imaging User’s Manual (PDF)” which is part of the Sapera LT software package.

To reduce the interrupt overhead in the host the following settings in the NIC are advised.

Packet Size

For a good 5Gigabit Ethernet connection with minimal packet resend conditions, host computer performance can generally be improved by increasing the data packet size. Each streaming video packet causes an interrupt in the host computer. Therefore increasing the packet size reduces the CPU overhead required to handle video data from the 5GigE Vision detectors.

A standard packet can have a size up to 1500 bytes. Many network cards support a jumbo packet mode that can extend that size up to 16Kbytes. In theory, a packet could be as large as 16 KB, but the CRC (cycle redundancy check) containing the checksum of each packet is not as efficient when the packet size grows larger than 9000 bytes. For this reason **we advise to set the packet size to 9014 bytes** (jumbo packet enabled).

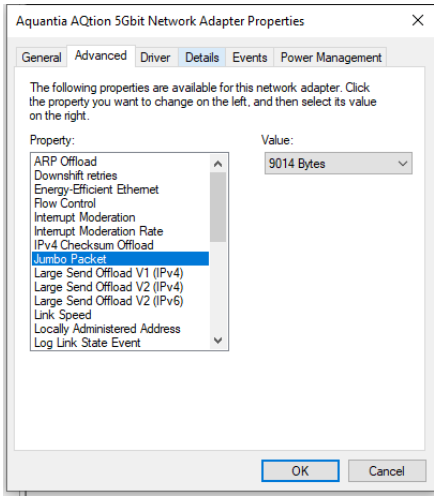

Some system and network card configurations may have difficulty streaming and handling jumbo packet data. If the system is having issues than it is advisable to disable the Jumbo Packet setting, and use standard size packets of 1500 bytes for your application.

Interrupt Moderation

Normally, each time a packet is received by the network card, the associated driver will receive an interrupt. Obviously, when the packet rate is very high (that is, at high transfer rate which is common for 5GigE Vision systems), this represents significant overhead. Most network cards have introduced an interrupt moderation mode where the card waits

to have received a certain number of packets over a maximum period of time before issuing the interrupt. This helps reduce the burden on the CPU as it can process multiple packets during the same interruption.

The 5Gbit adapter provides a configuration parameter to manually adjust the NIC interrupt moderation rate. By default the NIC driver sets this to Adaptive where the interrupt rate automatically balances packet transmission interrupts and host CPU performance. In most cases no manual optimization of the Interrupt Moderation Rate parameter is required.

In some conditions, video frames from the 5GigE Vision detector may be transferred to the host display or memory buffer as data bursts instead of a smooth continuous stream. The NIC may be over-moderating acquisition interrupts to avoid over-loading the host CPU with interrupts. If priority is required for acquisition transfers (i.e. a more real-time system response to the detector transfer) then the moderation rate should be set to "maximum" by manually adjusting the NIC parameter.

In the end, this is a compromise:

1. Enable interrupt moderation to minimize CPU usage, at the expense of a slight increase in latency (**recommended**).

2. Disable interrupt moderation to favor responsiveness of real-time system with a drawback in CPU usage.


In most situations, extra latency introduced by interrupt moderation is very low and thus the gain on CPU performance becomes more beneficial.

Receive Buffers

Under certain conditions the host PC system CPU may be busy with tasks other than the imaging application. Incoming image packets remain in the PC memory allocated to store packets instead of immediately being copied into the image buffer. By increasing the number of NIC (network interface card) receive buffers, more incoming image packets can be stored by the NIC before it must start discarding them. This provides more time for the PC to switch tasks and move image packets to the image buffer.

Not all network boards allow increases to their receive buffer count. Among those that do, different versions will have different maximum receive descriptor values.

We recommend **increasing the receive buffer size to the maximum permitted** by the network card, in order to provide more buffering capacity when needed.

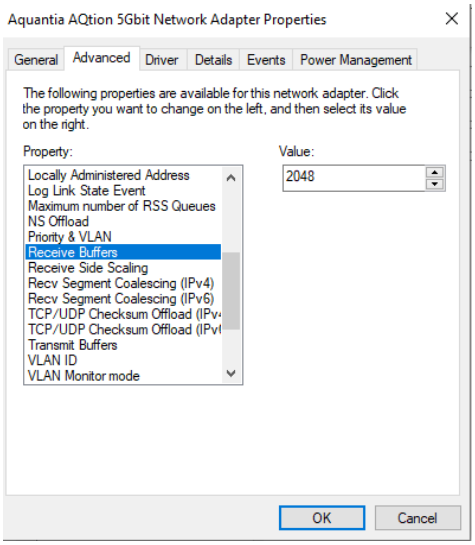

UDP Checksum Offload (IPv4)

Disable UDP Checksum Offload (IPv4).

Flow Control

The GigE Vision standard defines an inter-packet delay that can be used to manage flow control (i.e. the speed at which stream packet can be output to the network). This is useful when connecting multiple detectors to the same port of the network card, or when the network card/Ethernet switch (if used) is simply too slow to process those packets. A careful selection of equipment will ensure that the network equipment is fast enough to handle data transmitted to the wire-speed of 5 Gigabit per second. Therefore, inter-packet delay is typically only used when multiple detectors are connected to the same port of the network card, through an Ethernet switch.

It is important to consider that inter-packet delay inserts a minimum delay between image packets to spread packet transmission over a longer period of time. This can directly impact system latency as more time than could be necessary is put in between those packets. The best approach for real-time imaging is to dedicate a different network port to each detector. This way, the inter-packet delay can be eliminated in many cases.

Some network equipment also supports the optional IEEE802.3 PAUSE mechanism. This is a low-level handshake to ensure the receiver of the packets is not overwhelmed by the amount of data. It can propagate a pause signal back to the transmitter, asking to momentarily stop the data transmission (with a possible impact on the overall system latency). Again, by combining network equipment that can operate at wire-speed and allocating a different network interface port for each detector in the system, we can ensure these pause requests will not be used.

Connecting


1. After the install is complete, plug in the detectors communication cable.
2. Power up the detector.
3. After powering up the detector, the application automatically detects the detector. This may take 30 to 60 seconds. Wait until the detector connected indicator in the task bar (shown below) has confirmed that a connection has been established (the red cross over the camera icon disappears).



Checking detector status and information in Gigabit Ethernet

After the detector connection has been established, the status of the connection can be displayed by right clicking on the camera icon in the task bar and selecting "SHOW Status Dialog Box."


When you add or remove a detector from the network, it is automatically detected by the GigE server. A manual network scan can also be launched from this menu by selecting "Scan Network." This action will refresh the information of the device connected to the network. The "About Sapera GigE Server" option will display the version of the installed GigE driver.



Selecting the "*SHOW Status Dialog Box*" will open the device status window, which displays the basic information of the detector

- Serial Number
- Model Name
- MAC Address
- Packet size, which should be 9000
- Firmware version (build number)
- IP addresses of
    - Detector
    - Network Interface Card on host system to which the detector is connected

The default assigned detector IP address can be modified using the Teledyne DALSA Network Configuration Tool, which is part of the installation package.

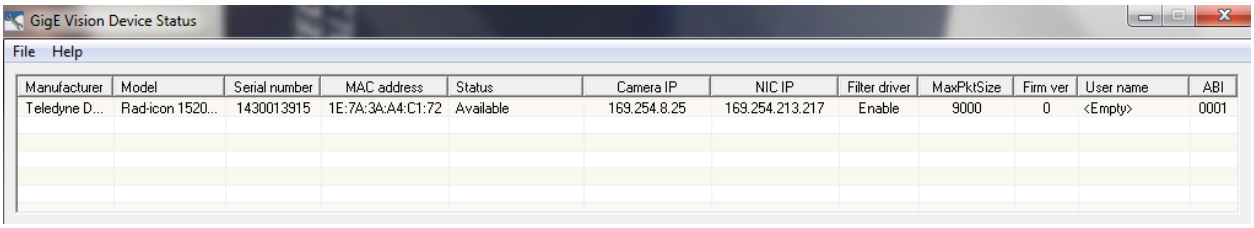

Quick Test with CamExpert

When the Shad-o-Scan detector is connected to a Gigabit network adapter on a host computer, testing the installation with CamExpert is a straightforward procedure.


- Start Sapera CamExpert by double clicking the desktop icon created during the Sapera LT software installation.
- CamExpert will search for installed Sapera devices. In the Device list area on the left side, the connected detector is shown or will be listed in a few seconds after CamExpert completes the automatic device search (device discovery).
- Select the Shad-o-Scan detector device by clicking on the camera user defined name. By default the Shad-o-Scan detector is identified by its serial number.
- Click on the Grab button for live acquisition (the Shad-o-Scan detector factory default is Free Running mode).
- See "Operational Reference" for information on CamExpert parameters with the Shad-o-Scan detector.
- The Snap or Grab function of CamExpert can be used to acquire live image. By default this will be dark signal from the sensor from the parameters pane a digital test pattern can be selected for testing network/computer bandwidth issues.
- Refer to the Teledyne DALSA Network Imaging package manual if error messages are shown in the Output Messages pane. But first, increase the value of the Interpacket Delay feature available from the GigE Vision TransportLayer Category group in CamExpert. An increase from default may correct errors with NIC interfaces that do not have adequate performance.

Acquiring Images

The CamExpert software can be started to acquire images.

Select the correct device from the Device Selection Menu.

The software will display all available device parameters of the detector.

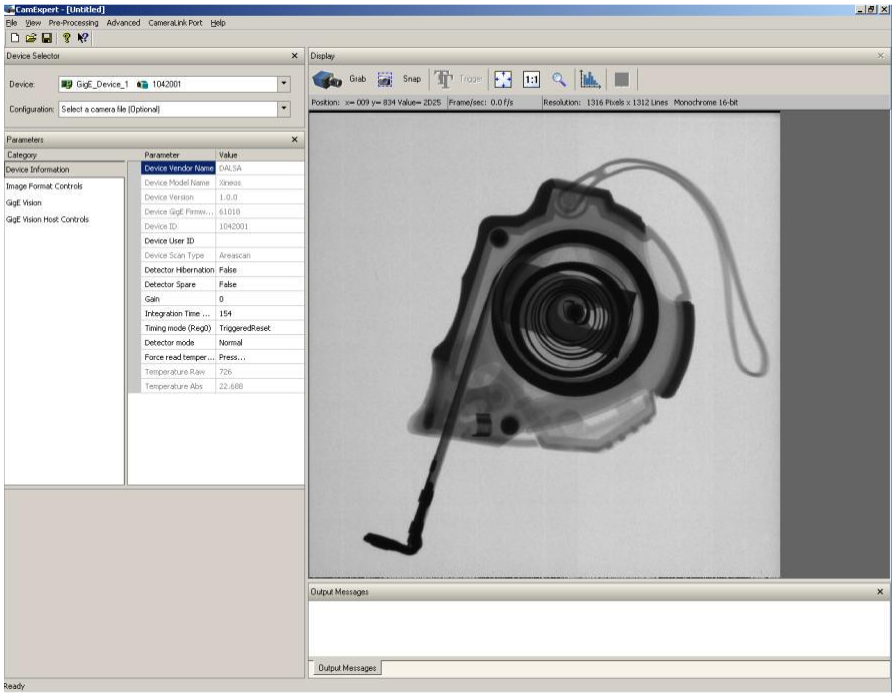

The user has the option to either snap an image or to grab continuously. Snapping an image produces a single frame, whereas the grabbing process generates multiple frames by operating in a continuous mode.

To snap an image:

Click the *Snap* button. The Detector has now snapped a single frame. The image appears in the GUI window.

To grab continuously:

Click the *Grab* button. The detector is now armed and ready to acquire images in continuous mode.

To stop a *Grab* process the user must press the *Freeze* button. After the *Freeze* button is pressed the detector ignores any additional triggers and no additional images are acquired.

5


Operational reference

Using CamExpert with the Shad-o-Scan Detector

The Sapera CamExpert tool is the interfacing tool for GigE Vision detectors and cameras, and is supported by the Sapera library and hardware. When used with a Shad-o-Scan detector, CamExpert allows a user to test most of the operating modes. Additionally CamExpert saves the Shad-o-Scan user settings configuration to the detector or saves multiple configurations as individual detector parameter files on the host system (*.ccf).


An important component of CamExpert is its live acquisition display window which allows immediate verification of timing or control parameters without the need to run a separate acquisition program.

Click on any parameter and a short description is displayed below the Category pane.

The same context sensitive help is available by clicking on the  button then click on a detector configuration parameter. Click on the  button to open the help file for more descriptive information on CamExpert.


CamExpert Panes

The various areas of the CamExpert tool are described in the summary figure below. GigE Vision device Categories and Parameter features are displayed as per the device's XML description file. The number of parameters shown is dependent on the View mode selected (Beginner, Expert, Guru – see description below).

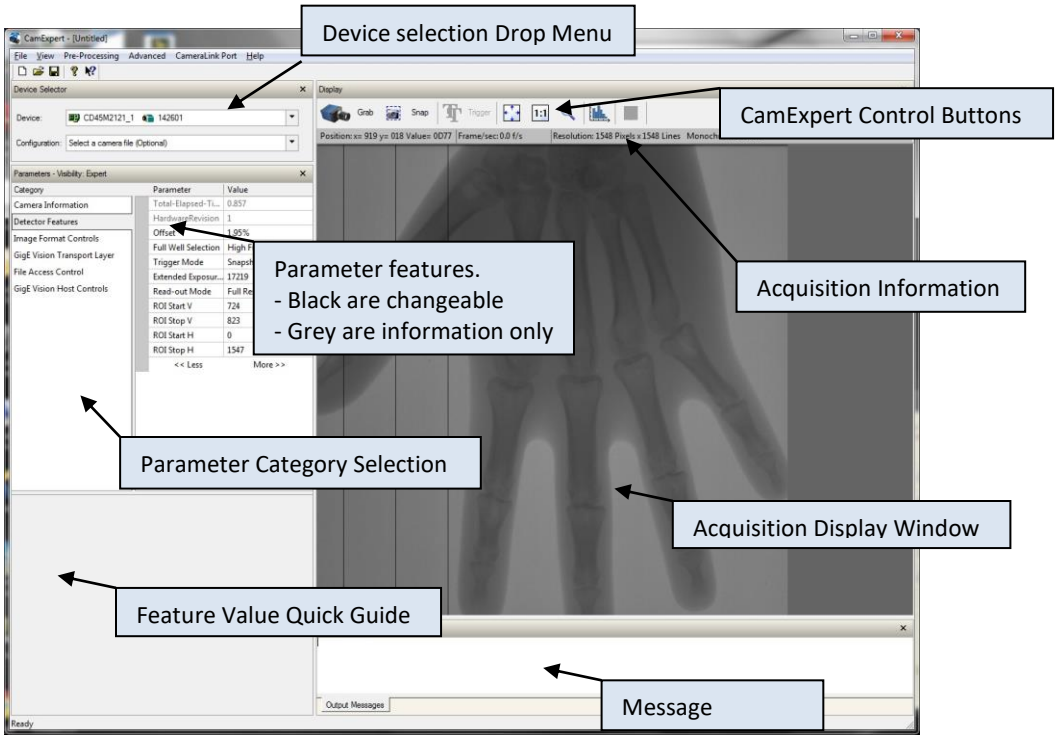

- **Device pane:** View and select from any installed GigE Vision or Sapera acquisition device. After a device is selected CamExpert will only present parameters applicable to that device.
- **Parameters pane:** Allows viewing or changing all acquisition parameters supported by the acquisition device. CamExpert displays parameters only if those parameters are supported by the installed device. This avoids confusion by eliminating parameter choices when they do not apply to the hardware in use.
- **Display pane:** Provides a live or single frame acquisition display. Frame buffer parameters are shown in an information bar above the image window.

- **Control Buttons:** The Display pane includes CamExpert control buttons. These are:

	**Acquisition control button:** Click once to start live grab, click again to stop.
	**Single frame grab:** Click to acquire one frame from device.
	**Software trigger button:** With the I/O control parameters set to Trigger Enabled / Software Trigger type, click to send a single software trigger command.
	**CamExpert display controls:** (these do not modify the frame buffer data) Stretch (or shrink) image to fit, set image display to original size, or zoom the image to any size and ratio. Note that under certain combinations of image resolution, acquisition frame rate, and host computer speed, the CamExpert screen display may not update completely due to the host CPU running at near 100%. This does not affect the acquisition.
	**Histogram / Profile tool:** Select to view a histogram or line/column profile during live acquisition.

- **Output pane:** Displays messages from CamExpert or the GigE Vision driver.

CamExpert View Parameters Option

All detector features have a Visibility attribute which defines its requirement or complexity. The states vary from Beginner (features required for basic operation of the device) to Guru (optional features required only for complex operations).

CamExpert presents detector features based on their visibility attribute. CamExpert provides quick Visibility level selection (Beginner/Expert/Guru) via controls below each Category Parameter list [<< Less More>>]. The user can also choose the Visibility level (Beginner/Expert/Guru) from the View - Parameters Options menu.


Camera Information

The following table describes the parameters Display Name as shown in CamExpert and their feature name, accessibility (RO=ReadOnly, RW=Read/Write, WO=WriteOnly) and description.

Display Name	Feature	Acc	Description
Manufacturer Name	DeviceVendorName	RO	Displays the device vendor name.
Family Name	DeviceFamilyName	RO	Display the device family name.
ModelName	DeviceModelName	RO	Displays the device model name.
Device Version	DeviceVersion	RO	Displays the device firmware version. This tag will also highlight if the firmware is a beta or custom design.
Device Product ID and Build number	DeviceProductIDBuild	RO	Provides the hardware Product ID and software Build Number
Hardware Revision	HardwareRevision	RO	Processing board hardware revision
Serial Number	DeviceID	RO	Displays the device's factory set camera serial number.
MAC Address	deviceMacAddress	RO	Displays the unique MAC (Media Access Control) address
Device User ID	DeviceUserID	RW	Feature to store a user-programmable identifier of up to 15 characters. The default factory settings is empty.
Device Reset	DeviceReset	WO	Resets the device to its power up state.
Power-up Configuration Selector	UserSetDefaultSelector	RW	Selects the camera configuration set to load and make active on camera power-up or reset. The camera configuration set are stored in camera non-volatile memory. (RW)
Factory Setting	*FactorySetting*		*Load factory default feature settings.*
UserSet1	*UserSet1*		*Select the user defined configuration UserSet 1 as the Power-up Configuration.*
UserSet2	*UserSet2*		*Select the user defined configuration UserSet 2 as the Power-up Configuration.*

Display Name	Feature	Acc	Description
User Set Selector	UserSetSelector	RW	Selects the camera configuration set to load feature settings from or save current feature settings to. The Factory set contains default camera feature settings.
Factory Setting	*FactorySetting*		*Select the default camera feature settings saved by the factory.*
UserSet1	*UserSet1*		*Select the User Defined Configuration space UserSet1 to save to or load from features settings previously saved by the user.*
UserSet2	*UserSet2*		*Select the User Defined Configuration space UserSet2 to save to or load from features settings previously saved by the user.*
Load Configuration	UserSetLoad	WO	Loads the camera configuration set specified by the User Set Selector feature, to the camera and makes it active
Save Configuration	UserSetSave	WO	Saves the current camera configuration to the user set specified by the User Set Selector feature. The user sets are located on the camera in non-volatile memory
Temperature	DeviceTemperature	RO	The temperature on the processing board in degrees Celcius

Camera Configuration Selection Dialog

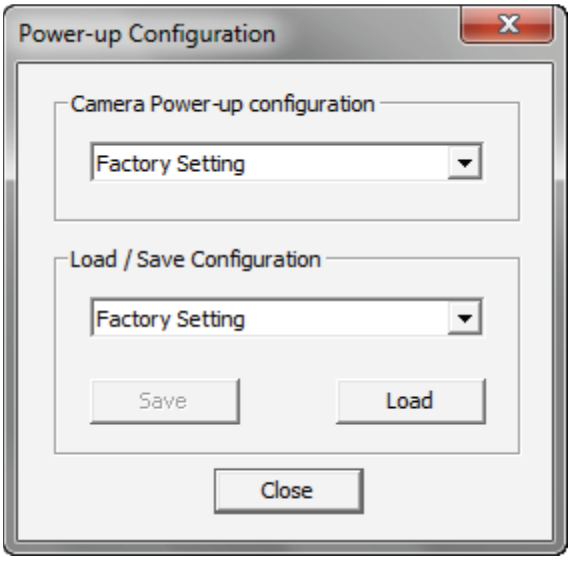

CamExpert provides a dialog box which combines the features to select the detector power-up state and for the user to save or load a detector state from memory.

Camera (Detector) Power-up Configuration

The first drop list selects the detector configuration state to load on power-up (see feature UserSetDefaultSelector). The user chooses from one factory data set or one of two possible user saved states.

User Set Configuration

The second drop list allows the user to change the detector configuration anytime after a power-up (see feature UserSetSelector). To reset the detector to the factory configuration, select Factory Setting and click Load. To save a current detector configuration, select User Set 1 or 2 and click Save. Select a saved user set and click Load to restore a saved configuration.

Note: A firmware reboot (power cycling) may be required after resetting the user set configuration to the Factory Setting.

Sensor Control

The Shad-o-Scan Detector controls, as shown by CamExpert, groups the detector-specific parameters. The features which are underlined link to the paragraph which describes these features in more detail.

Display Name	Feature	Acc	Description
Read-Out Mode	*Framerate*	RW	Framerate in Hz Trigger Mode off
	Exposure		Exposure time in us Trigger Mode off
Binning list	*Binning 1x1*		*Read the full array of the image sensor*
	Binning 2x1		*Bins in sensor vertically*
	Binning 2x2		*Bins in sensor vertically and digital in FPGA for horizontally direction*
	Binning 4x4		*Bins in sensor vertically and digital in FPGA for horizontally direction*
Trigger Mode Mode	TriggerModeTrigger Mode	RW	Controls by what source initiate and how the sensor read-out
off	*Synchronous*		*Detector uses internal timing*
on	*Trigger Source*		*Read-out of sensor occurs on falling-edge of trigger input*
Acquisition Frame Rate (in Hz)	Acquisition Frame Rate (in Hz)	RW	Framerate in Hz in Trigger Mode off
Exposure Time (in us)	ExposureTime	RW	Exposure time in us in Trigger Mode off
Offset	Offset	RW	Sensor dark ADC offset level; based on full scale of sensor
0%	*Offset0pct*		*0*
1.95%	*Offset1pct95*		*1,95% of 16384*
3.9%	*Offset3pct9*		*3.9% of 16384*
6.25%	*Offset6pct25*		*6.25% of 16384*
Full Well Selection	FullWell	RW	Selects the full well of the pixels in the sensor array
High Full Well	*HighFullWell*		*Large full well capacitor*
Low Full Well	*LowFullWell*		*Small full well capacitor (default)*
Horizontal Offset	*Horizontal Offset*	*RW*	*Horizontal start position for ROI mode; min 0, max 3072, multiple of 2*
Vertical Offset	*Horizontal Offset*	*RW*	*Vertical start position for ROI mode; min 1, max 64, multiple of 2*

Width	*Width*	*RW*	*Horizontal ROI size; min 0, max 3072, multiple of 2*
Height	*Height*	*RW*	*Vertical ROI size; min 16, max 64, multiple of 2*

Read-Out Mode

When the ExposureAlignment is set to Synchronous the framerate can be set using the acquisition mode framerate parameter.

Full Resolution

In this Read-Out Mode the full resolution of the sensor is read out and streamed to the host system.

Binning 2x1, 2x2, 4x4

The detector supports 2x1, 2x2 and 4x4 pixel binning.

Region of Interest

With Region of Interest (ROI) a region in the pixel array can be selected to read-out from the pixel array from the sensor and transferred to the host system as shown in the figure below.

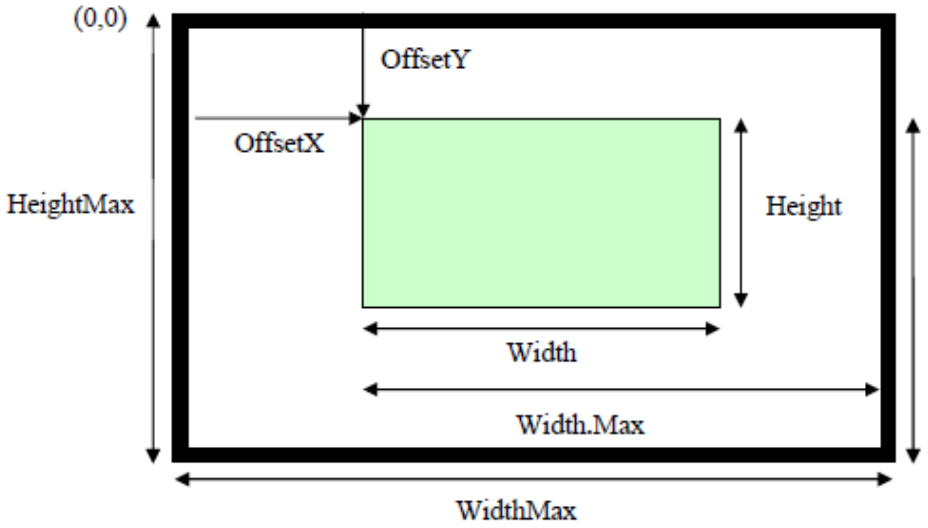


Figure Image size and defining a Region of interest

The sensor provides SensorWidth times SensorHeight pixels.

Within the shrunk image the user can set a Region of interest using the features OffsetX, OffsetY, Width, and Height. The resulting image generated by the device has Width time Height pixels. OffsetX and OffsetY are given with respect to the upper left corner of the image which has the coordinate (0, 0) (see Figure).


Trigger Mode

Synchronous Mode

In this mode the detector will run continuously on internal timing. No trigger input is required to initiate a frame read-out. The frame rate is determined by the time between successive frame read-outs which can be set by the Exposure or Framerate feature.

In this mode the sensor will integrate and read-out continuously even when the host does not acquire any images. However the trigger output is suppressed when no images are acquired, this is useful to see at what moment an integration period will be acquired and streamed to the host system.

When a grab is started the next integration period will be acquired and sent to the host system. If a grab is started but the sensor is still in the integration period this frame will be dropped and the following frame will be send to the host system; this to avoid changes to the sensor during the integration period (which can happen before acquiring images).

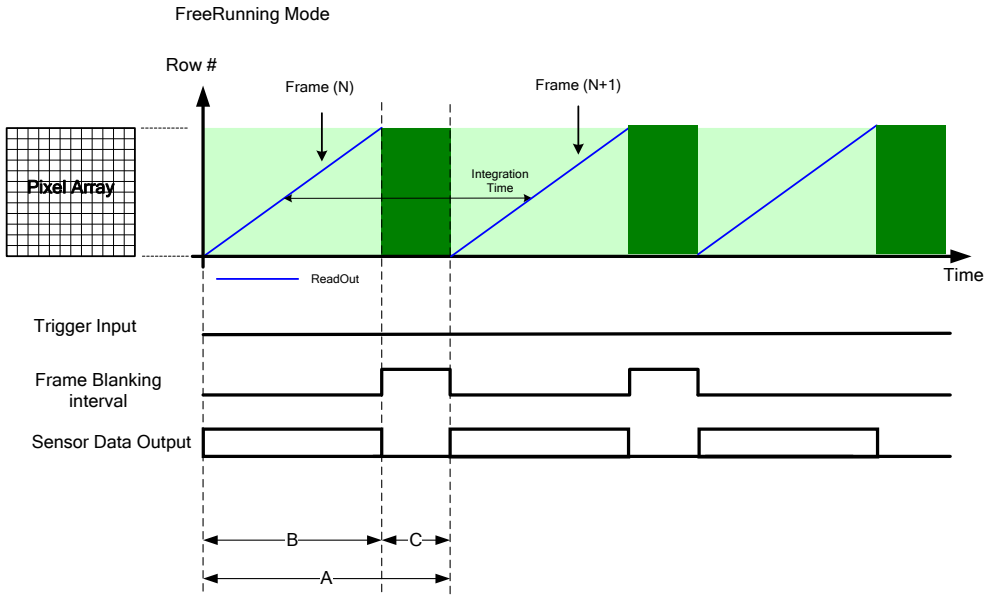

Operation mode	Full resolution	Binning 2x2
1/A: Frame rate	730 FPS	1390 FPS
A: integration time	1.36 ms	0.644 ms
B: readout time	1.36 ms	0.644 ms
C: Frame Blanking interval (A_B)	0.001 ms	0.001 ms


Figure timing diagram 'free running'

Triggered (External) Mode

In this mode the detector will take a single image at the moment a trigger signal is applied to the detector.

When using pulsed X-rays, the X-ray exposure including X-ray rise- and fall-times have to be within the "Exposure Time" window (C).

The trigger output indicates the Exposure Time window when no read-out of the sensor occurs.

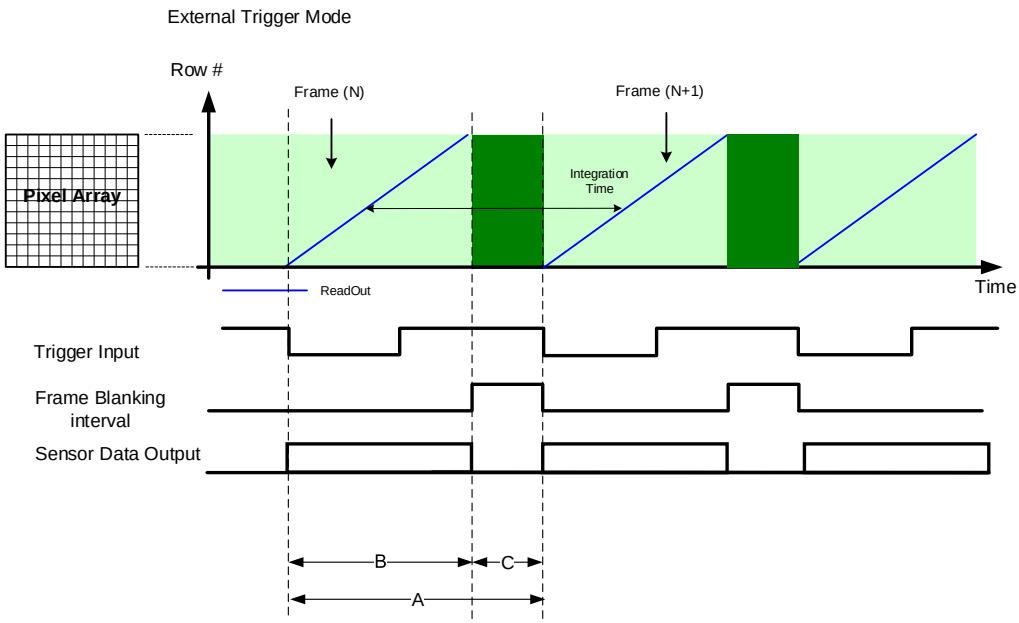

Operation mode	Full resolution	Binning 2x2
1/A: Frame rate = trigger frequency	730 FPS	1390 FPS
A: integration time	1.36 ms	0.644 ms
B: readout time	1.36 ms	0.644 ms
C: Frame Blanking interval (A_B)	0.001 ms	0.001 ms

Figure timing diagram 'Trigger Mode'

Image Format Control

The Shad-o-Scan Image Format controls, as shown by CamExpert, group parameters used that give information about the resolution and pixel format.

Display Name	Feature	Acc	Description
PixelFormat	PixelFormat	RO	Format of the pixel provided by the device. Contains all information as provided by PixelCoding, PixelSize combined in one single value
Pixel Size	PixelSize	RO	*Total Size in bits of an image pixel*
Mono	*Mono*		*Pixel is monochrome*
Width	Width	RO	Width of the Image provided by the device (in pixels)
Height	Height	RO	Height of the Image provided by the device (in pixels)

Image Processing Control

The following image (pre-)processing operations are considered standard practice in today's digital imaging applications, prior to distilling technical or clinical information through further image (post-)processing operations:

Defect Pixel Correction (DPC), in which defective or deviating pixels in the image are interpolated using information from neighboring pixels; and

Flat Field Correction (FFC), a combination of black (offset) and gain correction, in which spatial non-uniformities in the images due to detector or system (X-ray source, collimation) characteristics are corrected to reduce fixed pattern noise and optimize dynamic range.

The Rad-icon Detector controls, as shown by CamExpert, groups the image processing specific parameters. Defect Pixel Correction (DPC) and Flat Field Correction (FFC) functions are supported by the detector. The calibration reference maps required for DPC and FFC operations are loaded in the detector's non-volatile memory, for each *Readout*. A set of factory maps and a set of customer maps are available. The factory maps are read-only while the customer maps can be updated by the User.

The DPC and FFC functions can be used in combination with different *Trigger* and *Region of Interest* readout modes.

The function features are listed in the table below; the following paragraphs describe these features in more detail.

Display Name	Feature	Acc	Description	Factory default	Min	Max
FFC Enable	FFCEnable	RW	Turns On/Off Flat Field Correction	On	-	-
Off	Off		Off: Disabled	-	-	-
On	On		On: Enabled	-	-	-
FFC Processing	FFCActive	RO	Shows if FFC processing is enabled and activated	-	-	-
Not Active	Not Active		FFC processing not active	-	-	-
Active	Active		FFC processing active	-	-	-
FFC Mode	FFCMode	RW	Changes Mode for Flat Field	Normal	-	-

			Correction			
Normal	Normal		Default Flat Field Correction Mode	-	-	-
New Dark	New Dark		Writes New Dark for Flat Field Correction	-	-	-
FFC New Dark Weight	FFCNewDarkWeight	RW	Select Weight for Dark reference update	10	0	100
Dark Map Save to Flash	FFCNewDarkSaveFlashReq	RW	Save Dark Map to Flash	-	-	-
FFC NewDark Status	FFCNewDarkStatus	RO		-	-	-
Map Select	FFCMapSelect	RW	Select automatic or manual FFC map selection	Auto	-	-
Auto	Auto		Automatic set FFC maps	-	-	-
Manual	Manual		Manual set FFC maps	-	-	-
Factory/Customer Map Select	FFCFileSetSelectCustomerMode	RW	Indicates the mode of Customer or Factory map	Auto	-	-
Auto	Auto		Use customer maps if exist else factory maps	-	-	-
Customer	Customer		Force using customer maps	-	-	-
Factory	Factory		Force using factory maps	-	-	-
FFC Gain Map	FFCFileSetSelectGainMode	RW	Indicates the map of file Gain selection	-	-	-
Map 0 … 7	Map0 … 7		Gain Map 0 … 7	-	-	-
FFC Gain Map	FFCFileGainMap	RO	Shows if	-	-	-

Status	Status		selected Gain Map is valid			
Ok	Ok		No Error	-	-	-
Invalid FullWell	InvalidFullWell		Invalid FullWell	-	-	-
Invalid Resolution	InvalidResolution		Invalid Resolution	-	-	-
No Memory	NoMemory		No Memory	-	-	-
No File	NoFile		No File	-	-	-
Invalid Dark Map	InvalidDarkMap		Invalid Dark Map	-	-	-
Invalid Gain Map	InvalidGainMap		Invalid Gain Map	-	-	-
Undefined Error	UndefinedError		Undefined Error	-	-	-
Not Initialised	NotInitialised		Not Initialised	-	-	-
FFC Dark Map	FFCFileSetSelectDarkMap	RW	Indicates the map of file Dark selection	-	-	-
Map 0 … 7	Map0 … 7		Dark Map 0 … 7	-	-	-
FFC Dark Map Status	FFCFileDarkMapStatus	RO	Shows if selected Dark Map is valid	-	-	-
Ok	Ok		No Error	-	-	-
Invalid FullWell	InvalidFullWell		Invalid FullWell	-	-	-
Invalid Resolution	InvalidResolution		Invalid Resolution	-	-	-
No Memory	NoMemory		No Memory	-	-	-
No File	NoFile		No File	-	-	-
Invalid Dark Map	InvalidDarkMap		Invalid Dark Map	-	-	-
Invalid Gain Map	InvalidGainMap		Invalid Gain Map	-	-	-
Undefined Error	UndefinedError		Undefined Error	-	-	-
Not Initialised	NotInitialised		Not	-	-	-

			Initialised			
DPC Enable	DPCEnable	RW	Turns On/Off Defect Pixel Correction	On	-	-
On	On		On: Enabled	-	-	-
Off	Off		Off: Disabled	-	-	-
DPC Processing	DPCActive	RO	Shows if DPC processing is enabled and activated	-	-	-
Not Active	NotActive		DPC processing not active	-	-	-
Active	Active		DPC processing active	-	-	-
DPC Error Handling	DPCErrorHandling	RW	Changes Defect Pixel Correction Error Handling	SetWhite	-	-
Set Pixel to White	SetWhite		Set Pixel to White	-	-	-
Keep Original Pixel	KeepOriginal		Keep Original Pixel	-	-	-

Defect Pixel Correction

To enable Defect Pixel Correction, set the *DPC Enable* to *On* (default setting).
By means of *Factory/Customer Map Select* the selection of the active map can be influenced. When it's on *Auto,* Customer maps have priority if available else the Factory maps will be used. *DPC Processing* will show *Active* when a valid DPC map is in use.

Flat Field Correction

To enable Flat Field Correction, set the *FFC Enable* to *On* and the *FFC Mode* to *Normal* (default setting).

By means of *Factory/Customer Map Select* and *Map Select,* the selection of the active reference maps can be influenced. When both are on *Auto*, the 1st dark and gain map in the row which fits to the resolution and full well capacity setting will be selected. Customer maps have priority over Factory maps. When *Factory/Customer Map Select* is set to *Factory* or *Customer,* the selection will limited to those categories.

When *Map Select* is set to *Manual,* the active FFC Gain and FFC Dark map can be selected from a list of EIGHT maps (Map 0 – Map 7). Factory maps are stored in a fixed order. Customer maps can be organized to the user's preference. As an example, it is possible to

store three gain maps for different exposure situations in combination with two dark maps for use with different integration times.

FFC Gain Map Status and *FFC Dark Map Status* indicate if a valid map has been selected. *FFC Processing* will show *Active* when both a valid FFC Dark and FFC Gain map is in use.

The dark reference map can be updated using actual dark images from the detector, for example when capturing images with long integration time. To do so, set the *FFC Mode* to *New Dark* and perform an image *Snap*. The detector will output the requested image to the host application. In detector volatile memory, the captured image will be added to the current dark reference map using the *FFC New Dark Weight* value. The dark reference map stored in the detector's non-volatile memory, which is loaded on power-up, is not automatically updated. With *DarkMap Save To Flash* you may store this new dark reference to the Customer Dark map. *FFC NewDark Status* indicates when the save operation is finished.

Example 1: to update the actual dark reference map, for example to correct for changing detector temperature conditions, set *FFC New Dark Weight* to 20 and *Snap* a few dark images every 5-10 minutes.

Example 2: to create a fully new dark reference map, for example when the integration time is significantly changed, first set *FFC New Dark Weight* to 100 and *Snap* a dark image to overwrite the old dark reference map. Then set *FFC New Dark Weight* to 10 and *Snap* at least 32 dark images to average out the random noise in the dark image.

Ensure that the detector is not exposed to X-rays during capturing of new dark images, as this will significantly impact the usability of the updated dark reference map and the quality of the FFC operation.

Disable DPC while creating new or updated dark and gain reference maps for FFC. This will ensure that FFC will deliver optimal results.

Volatile memory space of the detector is limited. This may cause a Gain/Dark map selection issue with map 7 when all customer maps (map 0 – map 7) are used for Full Resolution modes.

After changing the *Factory/Customer Map Select* mode, the detector needs to transfer the selected Factory/Customer Maps to volatile memory. When this process is finished, the detector's network connection needs to be re-established.

FFC and/or DPC processing will be disabled in case not all reference maps for the selected mode are available or the wrong map is selected in *Manual Map Select* mode. The *FFC Processing* and/or *DPC Processing* field will show *Not Active.*

Defect Maps

Introduction


Defect pixel reference maps are stored in detector non-volatile memory. These maps contain information on the position of defective (or deviating) pixels, required for Defect Pixel Correction (DPC). These maps are detector-specific, and are generated during Teledyne DALSA factory calibration.

Separate defect pixel maps are available for different Readout- and Full Well modes. These maps are used by the detector to apply DPC on images, before streaming them over the data communications interface.

The defect map can be used by the host application to apply corrections for defect pixels in images captured from the detector. The host application may use the "Teledyne X-Ray Processing Library" functions to apply such corrections, or for the creation and uploading of new correction maps. This library and its API can be downloaded from the Teledyne DALSA FTP server (ftp.teledynedalsa.com) on request.

DPC Calculation

The pixel value after DPC correction is interpolated from an analysis of neighboring pixel values in a 5x5 kernel. Interpolation is performed in the direction in which the image content shows the least amount of change within this kernel.

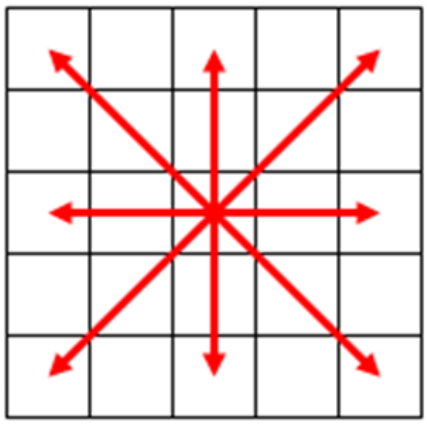


File Format

The file format of a defect map is as follows: A header indicates the specification of the defect map, and will be followed by a data block with the defect information per pixel. Only one bit per pixel is used to indicate the defect status (0 = no defect, 1 = defect). The defect status data per pixel is ordered row-by-row, left-to-right and top-to-bottom in an image displayed on a computer screen). The 32 bytes header format is described below:


Field	Description	Endian	Bytes
Header Version	0 Version number		2
Serial Number	Serial Number of Detector		16
CRC	CRC16 of total data file without the header	Little	2
Width	Number of columns (of full resolution image)	Big	2
Height	Number of rows (of full resolution image)	Big	2
File Type	0 Full Resolution, High Full Well 1 Full Resolution, Low Full Well 2 Binning 2x2, High Full Well	Big	2

	3 Binning 2x2, Low Full Well		
File Format	1 1 bit per pixel	Big	2
Extra1	Reserved	Big	2
Extra2	Reserved	Big	2

Example of defect map file header (hex format):

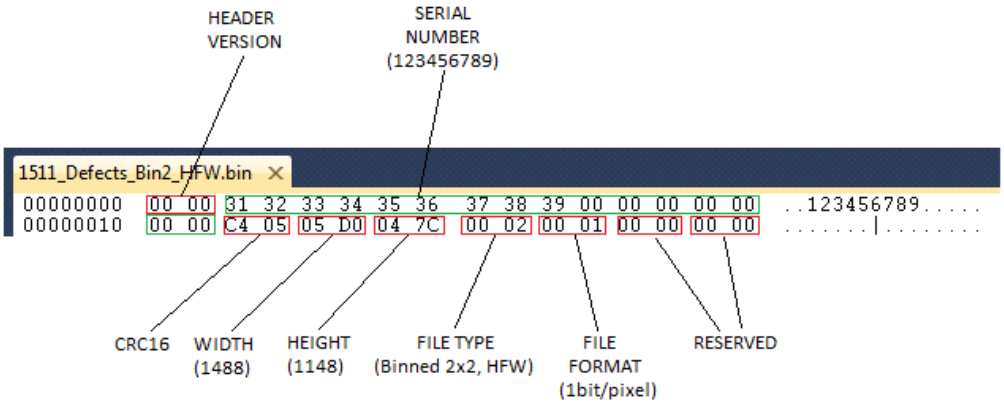

Up-, downloading and deleting

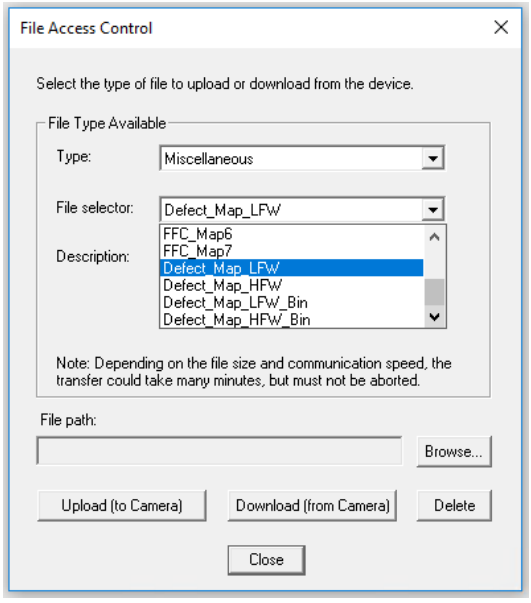

The File Access Control dialog box enables up-, downloading and deleting of defect map files.

Upload

To upload a customer defect map file from the host to the detector, the *Factory/Custom Upload* selector in the *File Access Control* menu has to be set to *Customer* before opening the *File Access Control* menu through *Upload/Download File*.
Select Type Miscellaneous in the first drop list and in the second drop list the Defect Map

with appropriate Resolution/Full Well mode. Press the *Browse…* button to select a defect map file on the host and press *Upload (to Camera)* to start the transfer to the detector. The upload will be confirmed with the message: **File Upload Completed**.

When attempting to upload a new defect pixel map, the detector will check the file header. In case the header is incorrect, uploading the file will be blocked with error message **The selected file write access to the device failed!**.

Delete

To delete a customer defect map file from the host, the *Factory/Custom Upload* selector in the *File Access Control* menu has to be set to *Customer* before opening the *File Access Control* menu through *Upload/Download File*.
Select Type Miscellaneous in the first drop list and in the second drop list defect map. Ensure yourself before pressing the *Delete* button, the selected file will be deleted immediately with the message: **File Deleted Successfully.**

Downloading

Both customer and factory Defect Maps can be downloaded. Set the *Factory/Custom Upload* selector in the *File Access Control* menu in the preferred position before opening the *File Access Control* menu through *Upload/Download File*.

To transfer a defect map file from the detector to the host press the button: *Download (from Camera)*. A browse screen will be opened to select the *Save as…* location on the host. Pressing the *Save* button after selecting the correct name and location, the detector will start a transfer of the defect map file of the selected Resolution/Full Well mode to the host. The download will finish with **The file download completed successfully** message.

Dark/Gain Maps

Introduction

Dark and Gain reference maps are stored in detector non-volatile memory. These maps contain information required for Flat Field Correction (FFC).

The Dark reference map is created without exposure to X-ray. The Gain reference map is calculated from dark-corrected images without object in the X-ray field.

Separate Dark and Gain maps are available for different Readout- and Full Well modes. These maps are used by the detector to apply FFC on images, before streaming them over the data communications interface.

The Dark and Gain maps can be used by the host application to apply offset and gain corrections to images captured from the detector. The host application may use the "Teledyne X-Ray Processing Library" functions to apply such corrections, or for the creation and uploading of new correction maps. This library and its API can be downloaded from the Teledyne DALSA FTP server (ftp.teledynedalsa.com) on request.

FFC Calculation

The pixel value after FFC correction, FFCVal(x,y), is given by the following formula:

$$FFCVal(x,y) = [PixelVal(x,y) - DarkVal(x,y)] * \frac{GainVal(x,y)}{2^{UnityGainFactor}} + Offset$$

FFCValue(x,y) Pixel value after FFC

PixelVal(x,y) Pixel value in raw image

DarkVal(x,y) Pixel value in Dark map


GainVal(x,y)	Pixel value in Gain map
UnityGainFactor	Value in map representing unity gain, as a power of 2
Offset	Fixed value added to prevent noise clipping

File Format

The file format of the dark (or gain) maps is as follows: a header indicates the specification of the map, and will be followed by a data block with the dark (or gain) information per pixel. The 32 bytes header format is described below:

Field	Description	Endian	Bytes
Header Version	1	Version number	1
File Type	1 Dark map		1
	2 Gain map		1
Serial Number	Serial Number of Detector		16
CRC	CRC16 of total data file without the header	Little	2
Width	Number of columns (of full resolution image)	Big	2
Height	Number of rows (of full resolution image)	Big	2
Image Format	0 Full Resolution		1
	1 Binning 2x2		1
Full Well	0 High Full Well		1
	2 Low Full Well		1
Data Format	2 2 bytes per pixel		1
Unity Gain Factor	0 for Dark map (20 = 1)		1
	12 for Gain map (212 = 4096)		1
Extra1	Reserved	Big	2
Extra2	Reserved	Big	2

Example of Gain map header (hex format:

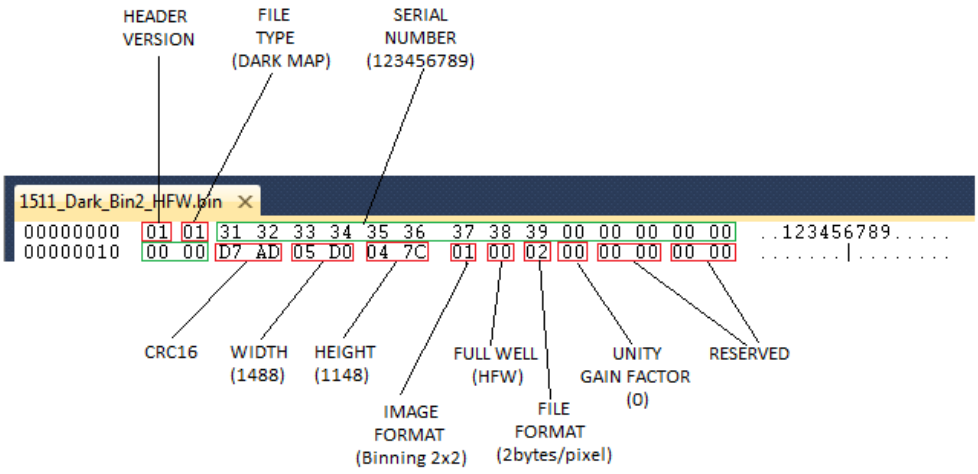


How to Create a New Gain Map

To use FFC to correct for system specific spatial intensity variations, new Gain maps should be created and uploaded to the detector as part of the factory system calibration routines.

For optimal gain correction, the Gain reference map should be created at an exposure of approximately 25% of the full scale output signal.


To create a new Gain map:

- Average at least 16 images captured by the detector, without any object placed in the X-ray beam.
- Subtract the average of at least 32 dark images, without X-ray exposure, using the same integration time (or frame rate) as used for capturing the X-ray images above.
- Determine the mean value of the image, in the region (ROI) where the signal value (X-ray exposure) is highest.

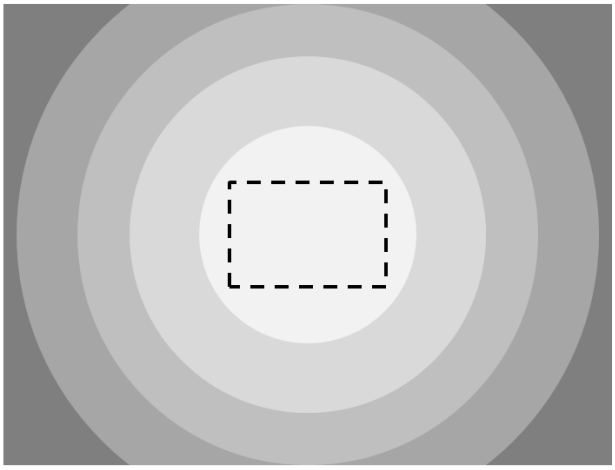

- For each pixel, divide this mean ROI value by the (averaged) X-ray exposed pixel value at that position (as floating point).
- Multiply the pixel values by 4096 (2^{12}), the Unity Gain Factor.
- Store the resulting pixel values (as 16-bit integer values) as the new Gain map, preceded by the appropriate file header information.

Up- , downloading and deleting

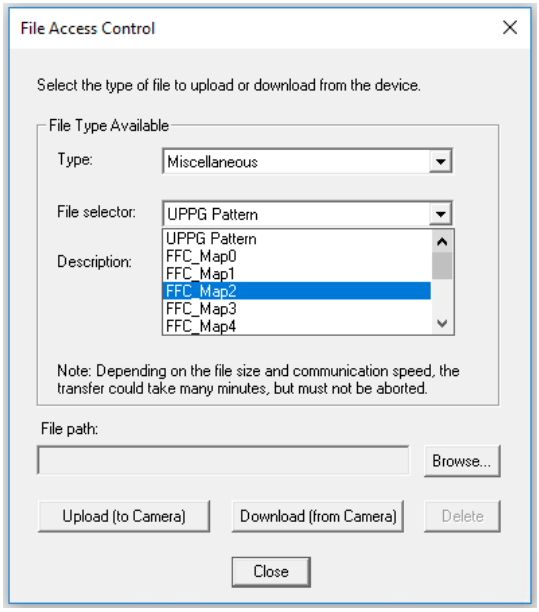

The File Access Control dialog box enables up- and downloading of dark/gain map files.

FFC_map0 till FFC_Map11 are the storage locations for Dark- and Gain Maps.
The Factory maps are stored in a fixed order. The file type per map is mentioned in the Description.
The Customer dark- and gain maps however can be stored in a random order.

Upload

To upload a customer gain- or dark map file from the host to the detector, the *Factory/Custom Upload* selector in the *File Access Control* menu has to be set to *Customer* before opening the *File Access Control* menu through *Upload/Download File*.
Select Type Miscellaneous in the first drop list and in the second drop list a FFC-Map. Press the *Browse…* button to select a dark/gain map file on the host and press *Upload (to Camera)* to start the transfer to the detector. The upload will be confirmed with the message: File Upload Completed.

Delete

To delete a customer gain- or dark map, the *Factory/Custom Upload* selector in the *File Access Control* menu has to be set to *Customer* before opening the *File Access Control* menu through *Upload/Download File*.
Select Type Miscellaneous in the first drop list and in the second drop list a FFC-Map. Ensure yourself before pressing the *Delete* button, the selected file will be deleted immediately with the message: File Deleted Successfully.

Download

Both customer and factory Gain- and Dark Maps can be downloaded. Set the *Factory/Custom Upload* selector in the preferred position before opening the *File Access Control* menu.


To transfer the selected FFC_map file from the detector to the host press the button: *Download (from Camera)*. A browse screen will be opened to select the *Save as…* location on the host. Pressing the *Save* button after selecting the correct name and location, the detector will start a transfer of the selected dark/gain map file to the host. The download will finish with The file download completed successfully message.

Firmware Update

Through the CamExpert file access control, a firmware update can be performed. Use the browse button to select a firmware file which has the extension CBF. The filename has the following format:

MODELNAMEFWVER.cbf

The modelname should be identical as the detector.

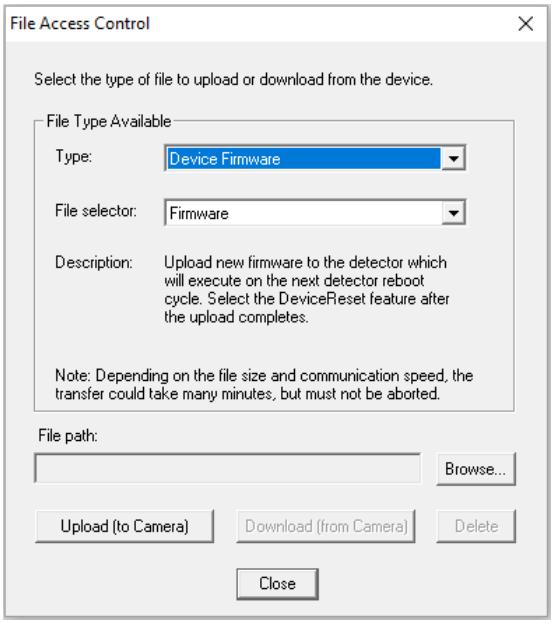

After uploading the file to the detector, CamExpert will request for a restart of the detector. This allows the reboot with the new firmware.

The timing control signals to the sensor of the detector are not part of the firmware but described in a separate file which is stored in the flash memory of the detector.
In some cases an update of this file is required.


The version can be seen in Camera Information > Timing Version:

Timing Version	4.3

This file can be uploaded through File Access Control > Upload/Download File.

Use the browse button to select a pattern file which has the extension BIN. The filename has the following format:

MODELNAME.bin

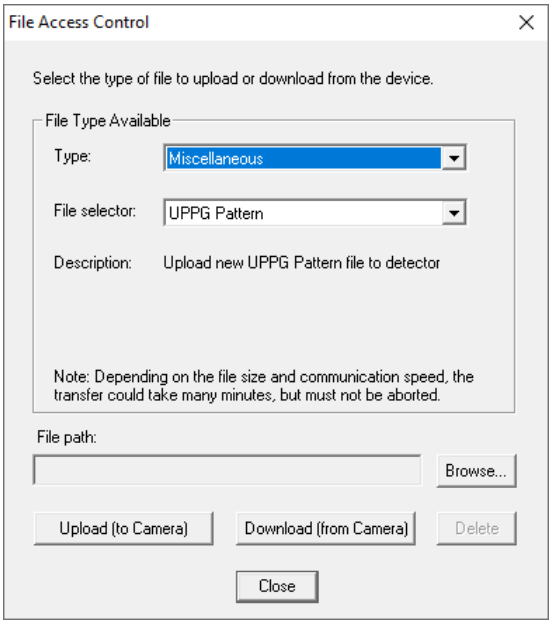
File Access Control
Select the type of file to upload or download from the device.
File Type Available
Type:
Miscellaneous
File selector:
UPPG Pattern
Description:
Upload new UPPG Pattern file to detector
Note: Depending on the file size and communication speed, the transfer could take many minutes, but must not be aborted.
File path:
Browse...
Upload (to Camera)
Download (from Camera)
Delete
Close

Shuttering

The Rad-icon Detector does not have a shuttering mechanism built into the detector. The detector can be operated quite normally with a continuous beam x-ray source, however there can be motion blur associated with continuous beam imaging. In the case that pulsed x-ray operation is required, the X-ray pulse must be carefully timed so that x-ray from the pulse are not incident on the detector during readout. This will cause imaging artifacts that show up as very uneven illumination within the images.

Dark Current after Standby

A first image acquired after long time in standby mode might contain unwanted signal. It is recommended to read and discard at least 2 images after standby.

Mode switches

A first image acquired after a change of mode might contain unwanted signal. It is recommended to read and discard one or more images at the start of a new measurement sequence.


When switching from free running to any other mode the detector may output still one image because the timing sequence was already started.


6


Mechanical Interface

Mechanical Dimensions


Shad-o-Scan 3001 Model

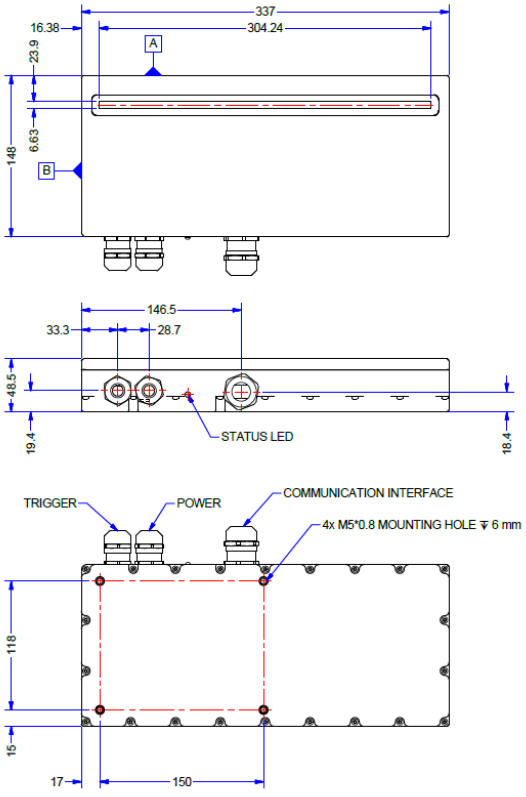





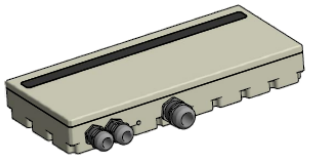

Shad-o-Scan 4501 Model

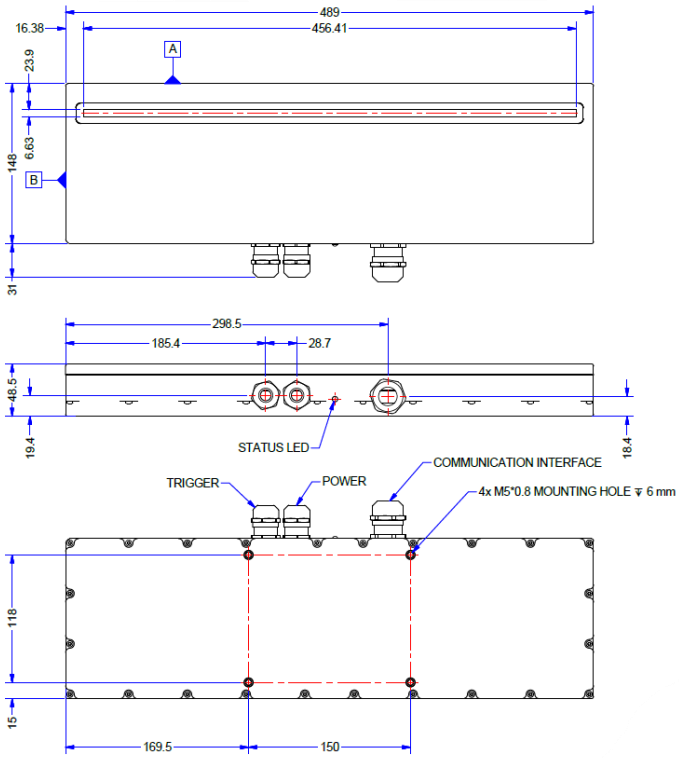



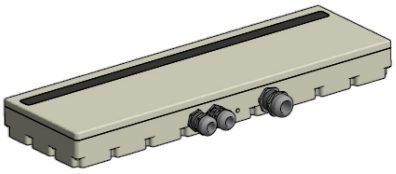

Appendix A

Revision History

Revision Number	Change Description	Revision Date
01	Draft release	July 6, 2020
01	First release	Sept 15, 2020