

MicroMix 5 Shaker User's Manual

Document number: 600885-0001

Revision A

Date: March 2007

Copyright © 2006 by Siemens Medical Solutions Diagnostics. All rights reserved.

Copyright © 2006 by Siemens Medical Solutions Diagnostics. All rights reserved.

This manual, and the software described in this manual, are copyrighted. No part of this manual or the described software may be copied, reproduced, translated or reduced to any electronic medium or machine-readable form without the prior written consent of Siemens Medical Solutions Diagnostics except that you may make one copy of the program CD solely for back-up purposes.

IMMULITE® is a registered trademark of Siemens Medical Solutions Diagnostics.
All other products mentioned are trademarks of their respective companies.



Siemens Medical Solutions Diagnostics
Certificate No: UQA0113493

Siemens Diagnostics' quality products are manufactured under a quality system that is registered to ISO 13485:2003.

Table of Contents

Table of Contents	3
1. Introduction	4
2. Performance Characteristics and Specifications	6
Technical Specifications	6
Mechanical Specifications	6
Environmental Specifications	7
Controller	7
Power Supply	7
3. Installation	8
Unpacking	8
Requirements	9
Setting Up	10
4. Principles of Operation	13
5. Control Panel	14
Function Key [Function]	14
Digit Control Keys [Right], [Left]	15
Start/Stop Key [Start/Stop]	15
6. Operating Instructions	16
Recommended Default Settings	17
RS232	17
7. Operating Precautions and Limitations	18
General	18
Operation	18
Defects and Abnormal Stresses	18
8. Hazards	19
Environmental	19
Electrical	19
9. Service and Maintenance	20
Sensor Test	20
Alarm Test	20
EPROM Software Version Display	21
10. Appendix: Forms	22
11. Technical Assistance	25

1. Introduction

The MicroMix 5 (Catalog number: **MMIX5**) is a fully programmable microplate and tube shaker. It allows complete control over the amplitude, frequency, direction of rotation and duration of shaking. The shaker has a capacity of four 96-well microplates, 120 tubes in one rack (Rack 513) or up to two racks (Rack 500) of 96 tubes, and can also shake tubes in foam racks.

This manual describes the installation, operation and maintenance of the MicroMix 5. Before operating the MicroMix 5, read this manual in its entirety, as it contains information necessary to ensure safe operation.

A set of preset shaking cycle patterns, called *Forms*, are stored in memory. The user can select from a range of variables in the **Form**, **Amplitude** and **Time** display modes to create an optimal **Mix** mode which suits a specific liquid viscosity and fill volume.

Not all tubes or wells in a microplate achieve resonance at the same frequency. Unlike most shakers, the MicroMix 5 shakes through a range of frequencies, ensuring that all tubes or wells in a microplate are mixed uniformly.

The MicroMix 5 consists of a base unit containing the control electronics, the electromechanics, a panel-mounted keypad and a Liquid Crystal Display (LCD). The base unit supports a lightweight but robust shaking table with plate-retaining strips, which can be exchanged for a mat and locators for shaking tubes.

The MicroMix 5 has a separate desktop power supply.



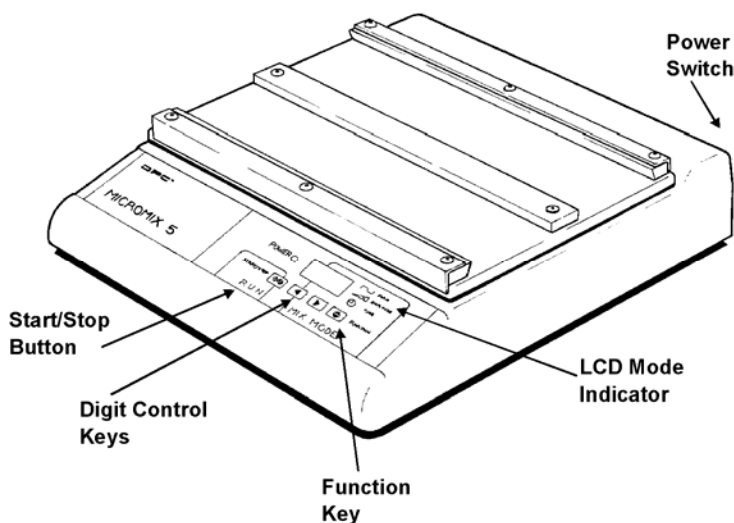


Figure 1: MicroMix 5 Shaker

Introduction (cont.)

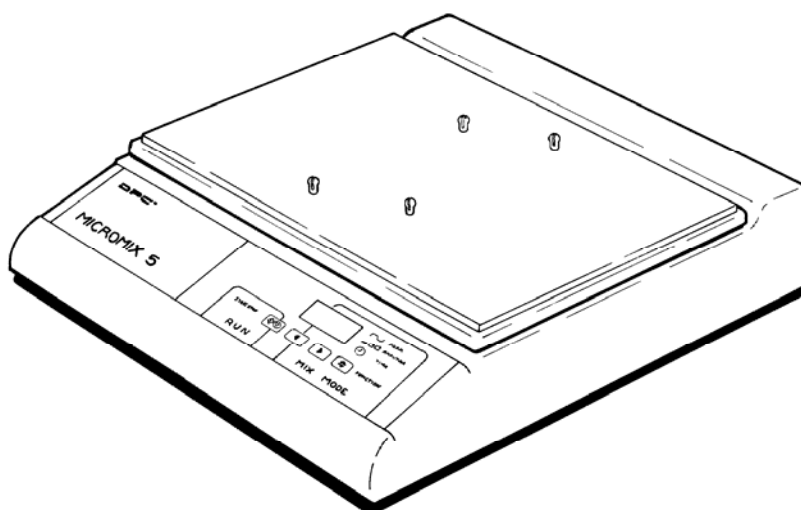

**Tube Racks
(RACK 500, RACK 513)**

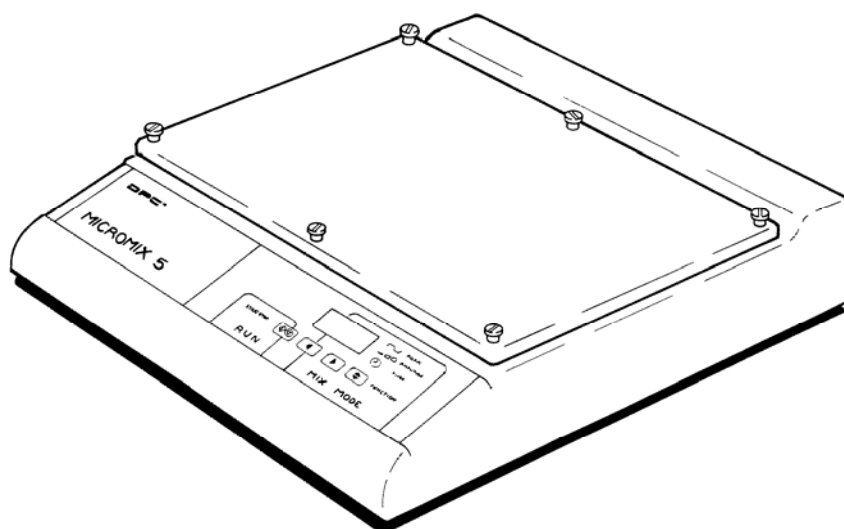

Foam Racks for Tubes

Figure 2: MicroMix 5 in Tube Shaking Configurations

2. Performance Characteristics and Specifications

Technical Specifications

The following are technical characteristics and specifications of the MicroMix 5:

- Maximum power consumption: 50 VA
- Power voltage: 90 – 260 VAC, 47 Hz – 63 Hz
- Power inlet at rear panel of power supply module
- Maximum peak-to-peak shake amplitude: 2.5 mm
- Shaking mode: horizontal plane, circular
- Shaker orbital speed range (frequency): 300 – 1800 rpm (5 – 30 cycles per second)
- Maximum capacity:
 - 4 microplates
 - 2 RACK 500 with 96 tubes per rack
 - 1 RACK 513 with 120 tubes per rack
 - 2 foam decanting racks with 100 tubes each
- Maximum shake mass:
 - 2 kg evenly distributed on shaking table from 5 Hz – 20 Hz
 - 0.5 kg evenly distributed on shaking table from 20 Hz – 30 Hz

Mechanical Specifications

The following are mechanical characteristics and specifications of the MicroMix 5. The mechanical and electrical components are fixed to a metal base plate. This is covered by a polyurethane foam case. The microplates are supported on an aluminum table. Other characteristics are:

- Footprint: 410 mm deep × 345 mm wide excluding power supply
- Height: 96 mm (overall height to seat of microplate)
- Weight: 6.7 kg; shipping weight: 8 kg

Vibration through the work surface is dampened by using feet made of special isodamped material.

Environmental Specifications

- Operating temperature: 0 to 40°C
- Storage temperature: -25 to 50°C
- Humidity: 10 to 90% RH, non-condensating
- RFC/EMI: Complies with EMC Directive 89/336/EEC
FCC 20780 Class B
VDE 0871 Level A

Controller

The controller comprises three main components:

1. Power inlet system, which consists of:
DC socket
Power switch
Interference suppression filter
2. Controller printed circuit board, incorporating front panel controls and indicators
3. Drive electromagnets

Power Supply

This is a modular bench-top switched mode power supply and features:

- International Electrotechnical Commission (IEC) inlet
- Fusing
- Interference suppression
- DC output cable and plug

3. Installation

Unpacking

Follow Figure 3 for unpacking instructions.

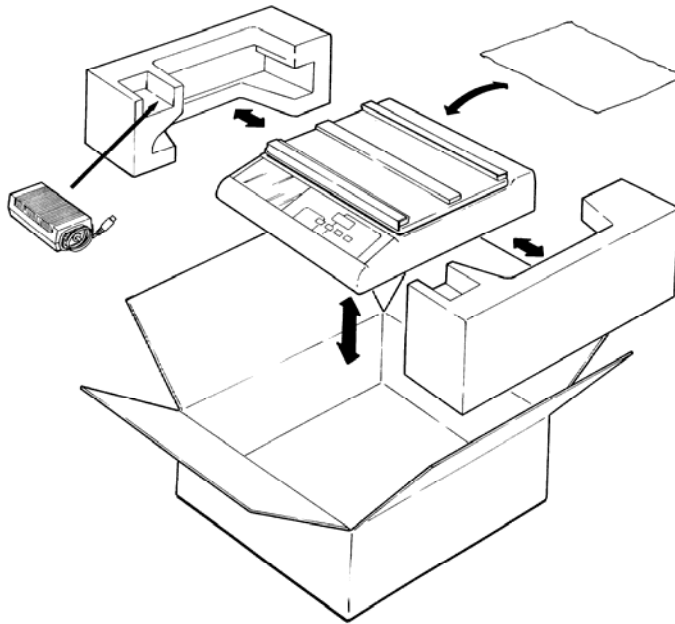


Figure 3: Unpacking

The main box should consist of the following:

- MicroMix 5 Shaker
- Bench-top power supply
- Power cord, appropriate to your country
- Black foam mat (MAT 25)
- MicoMix 5 Shaker User's Manual

The accessories pack should consist of the following:

- Five rack pillars
- Seven shoulder screws and washers
- Small allen key screwdriver

Requirements

Before plugging the external power supply into the Shaker and connecting to an appropriate outlet, ensure that the following requirements are met:

Site

The unit should be located on a level work surface free from strong sources of electromagnetic interference, e.g. centrifuge motors.

The proper work surface should measure as follows:

Height: 20 cm (8 inches)

Depth: 45 cm (18 inches)

Width: 36 cm (14 inches)

Power Supply

Only the supplied power supply should be used. The power supply unit accepts a supply voltage from 90 to 260 VAC and a frequency from 47 to 63 Hz. No adjustment is required.

CAUTION: This equipment requires connection to a properly grounded power source for safety reasons.

Setting Up

The MicroMix 5 may be reconfigured to shake microtiter plates, or tubes in racks or foams. The instrument is supplied preset to shake microtiter plates.

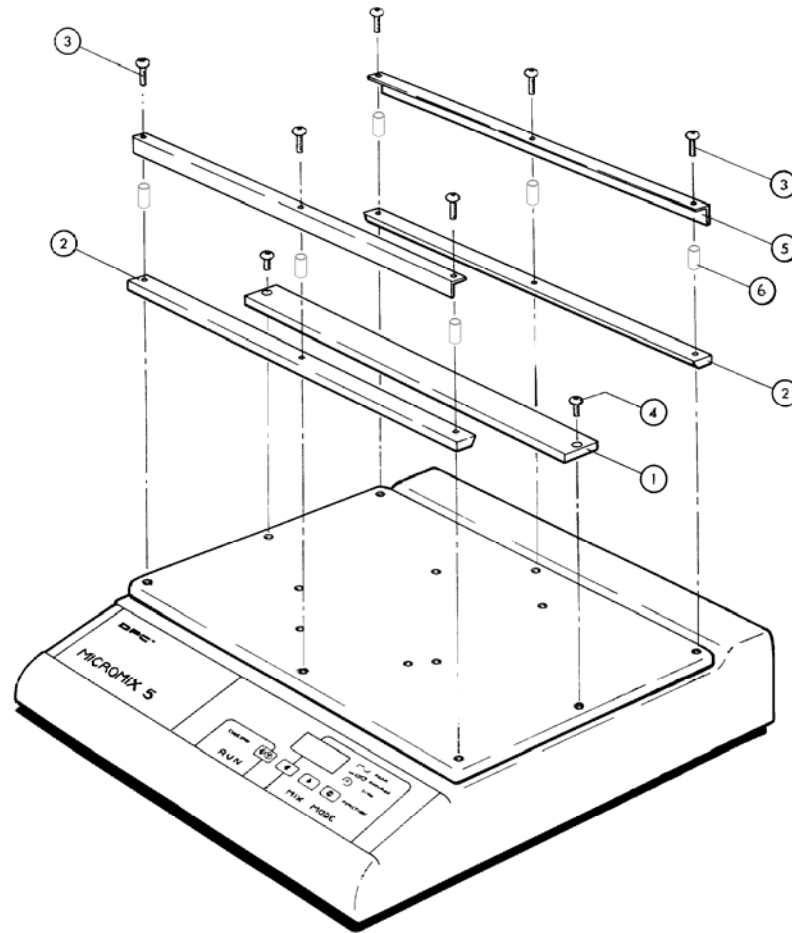


Figure 4: Microtiter Plate Shaking

Items Required

1. One perspex center strip
2. Two side foam strips
3. Six large allen screws
4. Two small allen screws
5. Two plastic strips
6. Six spacers
7. One small allen key screwdriver
(Item 7 is in the accessory pack.)

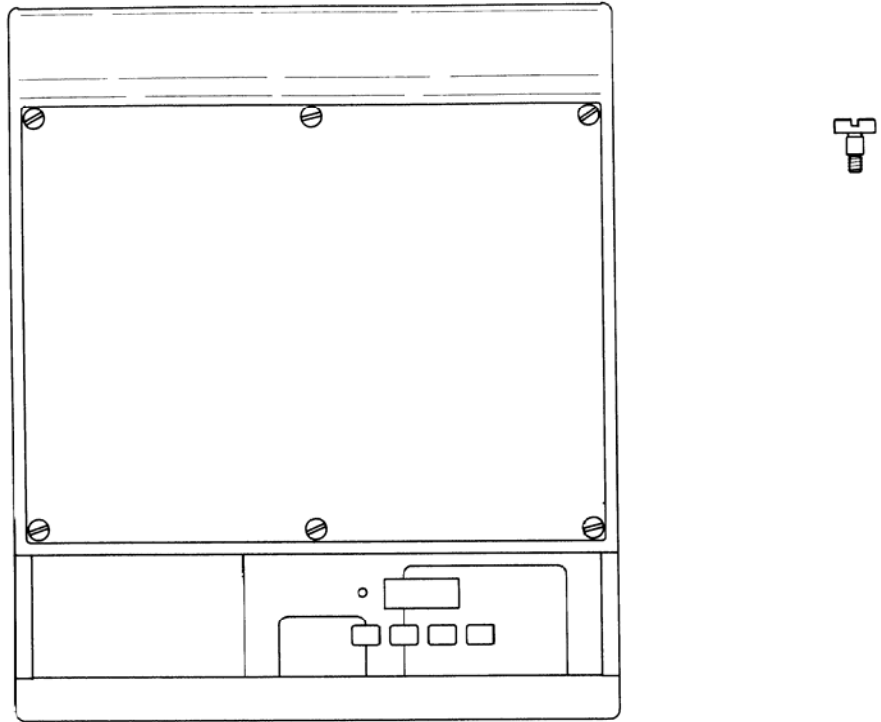


Figure 5: Tubes, Foam Shaking

Items Required

1. Six shoulder screws
2. One black foam Mat. MAT 25 (250 × 334 mm, 10 × 12.5 inches)
3. One small hex key screwdriver

Ensure that when fitting screws they are not cross-threaded into the shaker table top.

CAUTION: Do Not Overtighten the Screws

Setting Up (cont.)

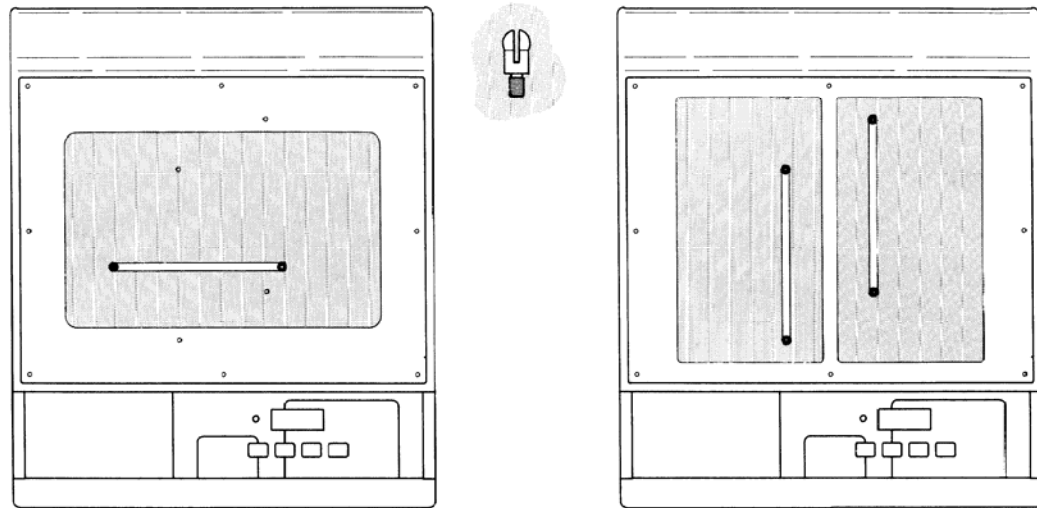


Figure 6: Tubes, Rack Shaking

Items Required

1. One black foam Mat. MAT 25 (250 × 334 mm, 10 × 12.5 inches)
2. Four rack pillars

When rack pillars are unused, they may be stored at the rear of the shaker. Caution must be exercised so as not to damage the threaded part of the pillars.

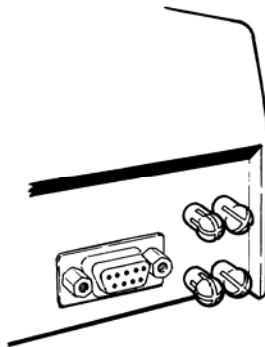


Figure 7: Rack Pillar Storage Location

4. Principles of Operation

Four diagonally arranged electromagnets fixed to the base are directed towards four pole pieces fixed to the shaking table. The electromagnets are activated and deactivated sequentially, so that the table shakes with an orbital motion. The table is mounted on rubber mounts, which ensure that the table moves only on a horizontal plane.

Motion is accurately controlled by a microcontroller. The amplitude is detected using a proximity sensor, and is maintained, regardless of the load, within the recommended operating range through dynamic feedback techniques.

The low inertia of the table enables the frequency and direction of mixing to be altered almost instantaneously. This also minimizes the reaction to the shaker body and transmission of vibration to the work surface.

The user may select one of a number of **Forms** and may also set the **Amplitude** and **Time** (duration of shaking). A total of 60 **Forms** are preset, with a subset of these optimized for plate shaking, tube shaking and constant speed shaking. The default shaker settings (**Form**, **Amplitude** and **Time**) selected when the shaker is switched **ON** may be reprogrammed by the user.

5. Control Panel

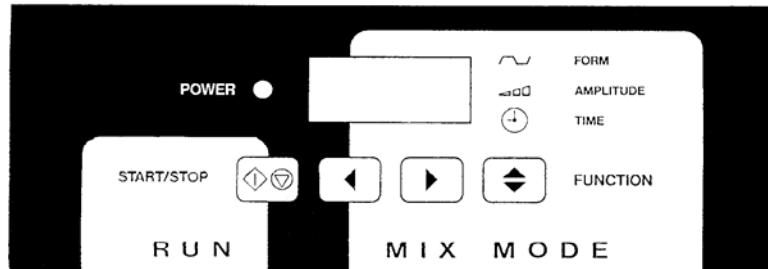


Figure 8: Control Panel

Legend



[Start/Stop]



[Left]



[Function]



[Right]

Function Key [Function]

The **[Function]** key is used to select any of three functions in which preset values may be chosen by the operator. The function selected is shown by the function indicator (appearing in the Mode Indicator window) which moves sequentially between **Form**, **Amplitude** and **Time** at each press of the key. The **[Function]** key also serves as a pause control in RUN mode with a toggle action. Key depression is acknowledged by a short audible "blip" unless the sounder is muted.

Form

The maximum number of **Forms** given with the MicroMix 5 is 60. **Form** value 60 sets the instrument to TIMER mode only.

Form affects the following:

- Speed Shake direction
- Rest period between changing directions

See the Appendix for further details.

Function Key (cont.)

Amplitude

The **Amplitude** selection ranges from 1 – 9, where 1 = minimum amplitude, and 9 = maximum amplitude

Time

The timer has a range of 1 – 199 minutes. The value counts down to zero from all nonzero values at the rate of 1 per minute after the **[Start/Stop]** key has been depressed. Setting **Time** to "0" places the instrument in continuous shaking mode. To stop continuous shaking, press the **[Start/Stop]** key.

See the Appendix for further details.

Digit Control Keys **[Right]**, **[Left]**

With the function indicator at the desired position, the **Form**, **Amplitude** or **Time** number as indicated in the LCD may be adjusted by means of the digit control keys as follows:

[Right] increases the value

[Left] decreases the value

A quick key depression changes the digit by one, while depressing the key longer than 0.7 seconds causes an acceleration through the numerical values. Digit wraparound is featured, i.e. each function returns to its minimum value after passing its maximum value.

Start/Stop Key **[Start/Stop]**

Shaking and/or timing is started by depressing and releasing this key, and may be stopped at any time by depressing the key again. As the time counts down, the function indicator flashes every 2 seconds.

When **Time = 0**, the alarm sounds and shaking ceases.

When the shaker/timer or alarm is stopped by this key, the READY mode is resumed with all the previously set parameters.

6. Operating Instructions

The power switch at the rear of the unit should be **OFF (O)** while connecting the power supply to the shaker. The DC power supply input may then be connected to the outlet.

1. Turn the power switch to **ON (I)**. The controller produces two short audible "blips"; the power ON indicator LED lights and the LCD panel indicate a number with the function indicator on **Form**.
2. The recommended **Form** and **Amplitude** settings should be selected and used for all assays, unless otherwise advised.

The **Time** setting should be adjusted according to assay instructions. This is done by pressing the **[Function]** key to select **Time**, and using the **[Right]**, **[Left]** keys to select the appropriate value in minutes.

The default **Time** setting, **0**, leaves the instrument in continuous shaking mode.

3. Press the **[Start/Stop]** button to begin shaking.
4. Shaking action may be paused by pressing the **[Function]** key while shaking is in action. The PAUSE mode is indicated by the function indicator set at **Time** flashing at approximately three times per second, and an audible warning consisting of 5 "ticks" per second.

In PAUSE mode, the timer is frozen and no power is applied to the shaker table. Shaking and time countdown (where applicable) resumes upon pressing the **[Function]** key a second time.

After switching the power **OFF (O)**, a minimum interval of 5 seconds should elapse before turning the power **ON (I)** again.

Sounder Mute

Switching the instrument **ON** while depressing the **[Left]** key mutes the sounder until the instrument is switched **OFF** and switched **ON** normally.

Resetting Power Up Setting

Switching the Instrument **ON** while depressing the **[Left]** and **[Right]** keys will enable the default settings at power up to be changed. Using the control panel, select the desired **Form**, **Amplitude** and **Time**. Pressing the **[Start/Stop]** key will start the shaker with these parameters, and permanently save them in internal memory (EPROM). The saving mechanism is then disabled, and any other function selected will not be saved.

When the instrument is subsequently switched **ON** it will default to the new settings. To save a new set of default parameters, the procedure must be repeated after switching on the instrument.

Recommended Default Settings

The recommended parameters to obtain various modes of shaking for assays are as indicated:

- For microtiter plate shaking, **Form 20, Amplitude 5** may be used. Other combinations may be considered as follows, **Form 8, 22, 21, 17, 20** – all at **Amplitude 5**.
- For shaking tubes in TUBE DECANTING Foams with Siemens Diagnostics assays use **Form 25, Amplitude 7**.
- For shaking tubes in RACK 500 or RACK 513 use **Form 24, Amplitude 7**.

NOTE: The shaker will not be able to maintain full shake amplitude with certain combinations of load, and selected **Forms** and **Amplitude** settings above 7. Do not exceed the mass, as stated in the Technical Specifications section.

RS232

There is an RS232 connector on the rear of the instrument to externally control the shaker.

For further information please contact your Siemens Diagnostics Distributor.

7. Operating Precautions and Limitations

General

Before operating the MicroMix 5, read this manual in its entirety, as it contains information necessary to ensure safe operation.

Control samples and calibrators supplied with *in vitro* diagnostic test kits should be processed by the MicroMix 5 in the same manner as test samples. Strictly follow the instructions in the package inserts provided by the manufacturer. **Do not use magnets or magnetized items except approved magnetic test tube racks near the equipment.** Protection from extremes of temperature and electrical interference is essential for proper operation.

The instrument should be unpacked and installed in accordance with the "Installation" section.

Operation

Ensure that the microplates are properly secured to the shaker platform before operating the MicroMix 5.

Ensure that the racks are properly seated on the shaker platform pillars before operating the MicroMix 5.

Ensure that foam decanting racks are properly affixed to the shaker platform before operating the MicroMix 5.

Do not exceed the maximum volume of 300 μ L per well in a standard 96-well flat-bottom microplate.

Defects and Abnormal Stresses

Whenever it is likely that the instrument's safe operation is compromised, it should be made inoperative and secured against any unintended operation.

The instrument's safety could be compromised, for example, if the instrument:

- shows visible damage
- fails to perform the intended functions
- has been stored for a long time under unfavorable conditions
- has been subjected to severe transport stresses

8. Hazards

Environmental

Infectious clinical samples and corrosive chemicals are commonly used with this equipment. Although the shaker is designed to avoid spillage under recommended working conditions, at higher amplitude settings spillage may occur; hand and eye protection and laboratory coats appropriate to the application should always be worn. If the shaker platform comes into contact with spilled liquid, it should be cleaned appropriately to avoid hazards.

Electrical

There are no USER SERVICEABLE PARTS within the MicroMix 5 and its power supply.

Never substitute a different cable for the power cord supplied with the instrument. The power cord should only be plugged into a power outlet with a proper ground.

The precautions for using any electrical equipment apply to this device. Do not use it during electrical storms. Do not touch switches or electrical outlets with wet hands. Switch the instrument **OFF (O)** before disconnecting.

9. Service and Maintenance

The MicroMix 5 is a highly reliable unit. This is achieved by the choice of well-proven components, the small number of moving parts, the minimal use of connectors and maximum use of digital techniques. The microcontroller, driver system, associated electronics and front panel controls and indicators are incorporated on a single printed circuit board.

There are no USER SERVICEABLE PARTS within the MicroMix 5. Authorized personnel only should carry out any necessary repairs to the unit, as these may involve the use of specialized equipment and fixtures.

The following diagnostic modes may be terminated and regular operation continued by depressing the **[Start/Stop]** key.

Sensor Test

Perform the following Sensor Test at 6-month intervals:

1. Switch the instrument **ON (I)** while depressing the **[Function]** key. This causes the LCD panel to indicate a value between 110 and 195 derived from the proximity sensor used for feedback control. The value on the LCD panel should be noted.
2. Move the shaking platform by hand in the horizontal plane. This causes the value to change on the LCD panel. When the shaking platform is resting in its equilibrium state, the value indicated should be between ± 10 of the previously indicated value. See item 1.
3. If the displayed value is outside the stated limits, contact your National Distributor for assistance.

Alarm Test

For this optional test, switch the instrument **ON** while depressing the **[Right]** key. This starts the alarm, which produces circular, sequential patterns on the LCD with a repeated audible tone of four short "blips" and one long "blip."

EPROM Software Version Display

Switch the instrument **ON (I)**, while keeping the **[Left]** and **[Function]** keys depressed. The EPROM software version is now displayed, e.g. 1.06. This is accompanied by a “chirping” sound. The mode may be terminated by pressing the **[Start/Stop]** key. The instrument is now ready for normal operation.

This feature is useful for checking the software version without having to remove the instrument's cover or controller board.

10. Appendix: Forms

The following table illustrates the available **Forms**. The MicroMix 5 offers a total of 60 preset **Forms**. Further details are available upon request from your distributor.

FORM	FRQ1 (Hz)	FRQ2 (Hz)	MODE	RAMP (Hz/sec)	GAP (sec)
1	5	30	2	0.12	1.0
2	5	10	2	0.13	1.0
3	7.5	12.5	2	0.19	0.9
4	10	15	2	0.25	0.8
5	12.5	17.5	2	0.32	0.7
6	15	20	2	0.39	0.6
7	17.5	22.5	2	0.44	0.5
8	20	25	2	0.50	0.5
9	22.5	27.5	2	0.50	0.5
10	25	30	2	0.50	0.5
11	5	10	3	0.13	1.0
12	7.5	12.5	3	0.19	0.9
13	10	15	3	0.25	0.8
14	12.5	17.5	3	0.32	0.7
15	15	20	3	0.39	0.6
16	17.5	22.5	3	0.44	0.5
17	20	25	3	0.50	0.5
18	22.5	27.5	3	0.50	0.5
19	25	30	3	0.50	0.5
20	20	25	3	7.0	0.2
21	20	25	2	1.75	0.3
22	20	25	2	0.25	0.5
23	8	11.5	2	0.10	1.0
24	11	14.5	2	0.10	1.0
25	13	18	2	0.10	1.0
26	8	11.5	3	0.10	1.0
27	11	14.5	3	0.10	1.0

Appendix: Forms (cont.)

Fixed Speed Forms

Form	FRQ1/FRQ2 (Hz)	MODE	Speed (RPM)
28	5	1	300
29	5	0	300
30	6.5	1	390
31	6.5	0	390
32	8.5	1	510
33	8.5	0	510
34	10	1	600
35	10	0	600
36	11.5	1	690
37	11.5	0	690
38	13.5	1	810
39	13.5	0	810
40	15	1	900
41	15	0	900
42	16.5	1	990
43	16.5	0	990
44	18.5	1	1110
45	18.5	0	1110
46	20	1	1200
47	20	0	1200
48	21.5	1	1290
49	21.5	0	1290
50	23.5	1	1410
51	23.5	0	1410
52	25	1	1500
53	25	0	1500
54	26.5	1	1590
55	26.5	0	1590
56	28.5	1	1710
57	28.5	0	1710
58	30	1	1800
59	30	0	1800
60	TIMER MODE		

Appendix: Forms (cont.)

Form Parameter Definitions

FRQ1: Start Frequency (orbital speed)

FRQ2: End Frequency ($\text{FRQ2} \geq \text{FRQ1}$)

Defining FRQ1 and FRQ2 sets up a range of shaking frequencies in Hz (cycles per second).

MODE

0 Constant direction, constant speed (clockwise).

1 Constant direction, constant speed (counter-clockwise).

2 Ramp frequency up, ramp frequency down, wait, change direction.

3 Ramp frequency up, wait, change direction, ramp frequency down, wait, change direction.

RAMP: Frequency ramp rate (speed of change from one frequency to the next through the range). Hertz per second.

GAP: Non-shaking period prior to change of direction. Seconds.

RPM: Speed of rotation for forms 0 and 1. Revolutions per minute.

Form 60

Selecting **Form** value 60 places the instrument in TIMER mode. No shaking takes place in this mode. The instrument counts down from a set time value, emitting an audible "tick" every second, while the function indicator blinks.

The display shows the time remaining until the alarm sounds.

Starting and stopping the TIMER mode is detailed in the "Start/Stop Key" section under "Control Panel."

Selecting **Form** 60 and setting the **Time** value to **0** activates the alarm immediately.

If the sounder has been muted, no seconds will be heard "ticking" during the TIMER mode, nor will there be an audible alarm when the time runs out.

11. Technical Assistance

For questions regarding the MicroMix 5 and its operation, or for service, contact Technical Service at Siemens Diagnostics or your National Distributor.

Tel: 973.927.2828

Fax: 973.927.0697