

Agilent Bravo Automated Liquid Handling Platform: 96-Channel 250 μ L Tip Accuracy and Precision

Technical Overview

Summary

- Bravo, 96LT head, 250 μ L tips
- 2 μ L: 2.1% CV \pm 3.3% accuracy
- 5 μ L: 1.1% CV \pm 0.3% accuracy
- 10 μ L: 1.0% CV \pm 4.2% accuracy
- >10 μ L: equal or better than 10 μ L CV & accuracy

Introduction

Automated liquid handling devices are used in many processes performed in laboratories today. Liquid handling automation increases sample processing and throughput¹ and improves accuracy (desired dispensed volume is equal to the actual dispensed volume) and precision (a narrow distribution of dispensed volume) when compared to a person operating a handheld liquid pipettor. Automated liquid handling devices can also significantly reduce the occurrence of errors in a process.² To further the effort to automate routine laboratory processes, Agilent Automation Solutions has developed the Bravo Automated Liquid Handling Platform.

Bravo Features

The Bravo has nine deck positions which accommodate any 96-, 384-, or 1536-well SBS standard microplates. Deck positions can be configured with heating, cooling, and shaking stations, as well as maintaining open locations for tip boxes, sample microplates, and reservoirs.

The Bravo can be used with 8-, 16-, 96-, or 384-channel fixed tip or disposable tip heads. Heads can be interchanged in a

matter of seconds. The Bravo is designed to be used either standalone or as part of a robotic laboratory automation system. It is also designed to fit inside some models of laminar flow hoods and retain laminar flow, thereby opening up cell-based plating and cellular assays to an automated liquid handling platform.

Accuracy and Precision Testing

This technical overview describes a method to measure the accuracy and precision of the Bravo in conjunction with a 96-Channel LT Disposable Tip Head at the lower end of the practical volume range (1-5 μ L). Performance at volumes >5 μ L meets or exceeds the 5 μ L performance. Measurements are determined by dispensing a tartrazine/DMSO solution into dry microplates, filling the plates with water, and measuring tartrazine absorbance. The product's performance meets or exceeds CVs of 5% and accuracy of $\pm 10\%$ of the desired volume across the practical volume range.

Materials

- Bravo with a 96-Channel LT Disposable Tip Head
- Agilent 96LT 250 μ L tips (product no. 19477-002)
- Agilent 96-well manual fill reservoir (product no. 08105-001)
- 384-well polystyrene, flat bottom plates (Greiner 781101)
- Tartrazine solution, 0.25% (w/v) dissolved in dimethylsulfoxide (DMSO)
- UV/Vis Spectrophotometer with a 405 nm filter (Thermo Multiskan Ascent)



The Agilent Bravo has nine deck positions and can be configured with interchangeable 8-, 16-, 96-, or 384-fixed and disposable tip heads.



Agilent Technologies

Method

60 mL of tartrazine solution is poured into a 96-well manual fill reservoir. The reservoir is placed on position 2 of the Agilent Bravo. A 250 μ L tip box is placed on position 3. A 96-well polystyrene plate is placed on position 5. VWorks4 liquid classes for 2, 5, and 10 μ L dispenses are utilized. A VWorks4 protocol is created and run in the following manner:


1. Tips are pressed onto the head.
2. 2.0, 5.0 or 10.0 μ L tartrazine solution is aspirated from the 96-well manual fill reservoir. Aspirate parameters are 5 mm from the bottom of the plate, and preceded by a 2 μ L pre-aspirate volume.
3. 2.0, 5.0 or 10.0 μ L tartrazine solution is dispensed into the 384-well plate. Dispense parameters are 0.2 mm from the bottom of the plate, and followed by dispensing a 2 μ L blowout volume.

Dispensed volumes are diluted to 50 μ L by the addition of water (in this case, with clean tips and a separate VWorks4 protocol). Plates are centrifuged at 1800 rpm for 60 sec to ensure full mixing and consistent well menisci. Absorbance is read at 405 nm.

Accuracy is calculated based on an equation derived from a tartrazine/DMSO calibration curve consisting of data points at 0.15, 0.32, 0.63, 1.25, 2.5, 5, 10, and 20 μ L, compared to the actual absorbance value in each well. Absorbance values in each well are used to determine the precision of the dispense. Coefficient of Variance (CV) calculations were made by dividing the standard deviation by the mean. The accuracy and precision results are typical, based on averages of three successive plate dispenses and readings. Accuracy outliers are an average per plate. Results may vary, depending on individual experimental methods and liquid class optimization.

Results

Volume (μ L)	2	5	10
Precision (% CV)	2%	1%	1%
% Accuracy (\pm)	3.3	0.3	4.2
Outliers (5%)	6	0	0
Outliers (10%)	0	0	0
Transfer time (seconds/plate)	22	22	37

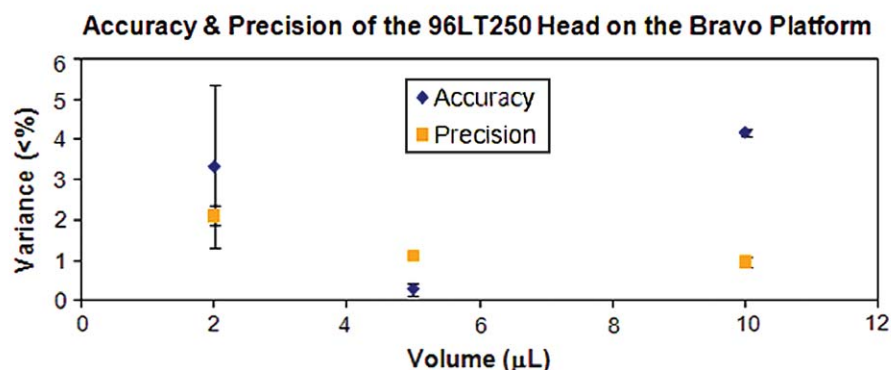

Conclusion

In summary, the liquid handling capabilities of the Bravo Automated Liquid Handling Platform in conjunction with a 96-Channel LT Disposable Tip Head provides precise, accurate and consistent liquid transfers. The 96-channel head can pipette across a wide volume range (1-250 μ L), allowing the automation of different processes using one head type. The highly configurable deck of the Bravo Automated Liquid Handling Platform along with its compact footprint makes it ideal for many applications in the laboratory including compound sample transfers, genomic applications, cell plating, and cell-based assays.

References:

1. M. J. Sofia, "Leveraging Compound Management Capabilities in Support of Drug Discovery: From Sample Archive to

Sample Distribution — Driving Efficiency and Improving Productivity," Laboratory Robotics Interest Group Meeting Oral Presentation, **2005**.

2. J. W. Holman, T. E. Mifflin, R. A. Felder, L. M. Demers, "Evaluation of an automated preanalytical robotic workstation at two academic health centers," *Clin. Chem.* 48:540-548, **2002**.

www.agilent.com/lifesciences/automation

This item is intended for Research Use Only. Not for use in diagnostic procedures. Information, descriptions, and specifications in this publication are subject to change without notice.

Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

© Agilent Technologies, Inc. 2010
Published in the U.S.A. June 24, 2010
5990-5904EN



Agilent Technologies